ARTISAN®
TECHNOLOGY GROUP

Your **definitive** source for quality pre-owned equipment.

Artisan Technology Group
(217) 352-9330 | sales@artisantg.com | artisantg.com

Full-service, independent repair center
with experienced engineers and technicians on staff.

We buy your excess, underutilized, and idle equipment
along with credit for buybacks and trade-ins.

Custom engineering
so your equipment works exactly as you specify.

- Critical and expedited services
- In stock / Ready-to-ship
- Leasing / Rentals / Demos
- ITAR-certified secure asset solutions

Expert team | Trust guarantee | 100% satisfaction

All trademarks, brand names, and brands appearing herein are the property of their respective owners.

Find the *Keysight / Agilent 53131A* at our website: ***Click HERE***

Agilent 53131A/132A/181A Counters

High-performance, low-cost counters simplify and speed systems and bench frequency measurements

Data Sheet





- 225 MHz bandwidth (optional 1.5, 3, 5, or 12.4 GHz)
- 10- or 12-digit resolution with 1 s gate time
- GPIB interface and IntuiLink connectivity software standard
- Data transfer rate of up to 200 fully formatted measurements/second

A family of universal and RF counters to meet your needs

Agilent Technologies 53131A/132A/181A high-performance counters give you fast, precise frequency measurements at an affordable price. These counters feature an intuitive user interface and one-button access to frequently used functions so you can make accurate measurements quickly and easily.

Agilent Technologies

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Real-time digital signal processing technology is used to analyze data while simultaneously taking new readings, speeding measurement throughput. The technology, developed for Agilent's high-end line of modulation domain analyzers, allows the counters to gather more data for each measurement, so you get higher-resolution measurements in a fraction of the time it takes other counters.

The 53131A/132A/181A counters offer built-in statistics and math functions so you can scale measurements and simultaneously measure and track average, min/max and standard deviation. Automated limit testing lets you set upper and lower limits for any measurement. An analog display mode lets you see at a glance whether a measurement is within pass/fail limits. The counters flag out-of-limit conditions and can generate an output signal to trigger external devices when a limit is exceeded. For quick access to frequently used tests, a single keystroke recalls up to 20 different stored front-panel set-ups.

For computer-controlled systems applications, each counter includes a standard GPIB interface with full SCPI-compatible programmability and a data transfer rate of up to 200 fully formatted measurements per second. The standard RS-232 talk-only interface provides printer support or data transfer to a computer through a terminal-emulation program.

Agilent 53131A Universal Counter
The two-channel 53131A counter offers 10 digits per second of frequency/period resolution and a bandwidth of 225 MHz. Time interval resolution is specified at 500 ps. An optional third channel provides frequency measurements up to 3 GHz, 5 GHz, or 12.4 GHz. Standard measurements include frequency, period, ratio, time interval, pulse width, rise/fall time, phase angle, duty cycle, totalize, and peak voltage.

Agilent 53132A Universal Counter
For applications requiring higher resolution, the 53132A offers the same features and functions as the 53131A, with up to 12 digits/sec frequency/period resolution and 150 ps time interval resolution. In addition, the 53132A offers advanced arming modes for time interval measurements.

Agilent 53181A RF Counter
Optimized for RF applications, the single-channel 10 digit/s 53181A measures frequency, period and peak voltage. A digit-blanking function lets you easily eliminate unnecessary digits when you want to read measurements quickly. For higher-frequency measurements, choose an optional second channel that provides measurements up to 1.5 GHz, 3 GHz, 5 GHz, or 12.4 GHz. A self-guided shallow menu makes this counter exceptionally easy to use.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Agilent IntuiLink provides easy access to the counter's data from your PC
The Agilent 53131A/132A/181A counters, capture precise frequency and time measurements. IntuiLink software allows that data to be put to work easily. You work in a familiar environment at all times, using PC applications such as Microsoft Excel® or Word® to analyze, interpret, display, print, and document the data you get from the counter.

It gives you the flexibility to configure and run tests from your PC making data gathering more convenient.

Agilent IntuiLink lets you:

- configure tests, including measurement type, number of readings, measurement speed, and more.
- choose display modes from real-time strip chart, histogram, readout, and table mode.
- scale measurements data.
- copy captured data to other programs.

Optional timebases offer increased stability
Optional timebases are available for 53131A/132A/181A counters to increase measurement accuracy. Option 010 provides a high stability oven timebase with aging of less than 5×10^{-10} per day.

1-year warranty
Each counter comes with operating, programming and service manuals, IntuiLink software, a power cord and a full 1-year warranty.

Time Base

Internal Time Base Stability (see graph 3 for timebase contribution of measurement error)

		Standard (0° to 50°C)	**Medium Oven** (Option 001)	**High Oven** (Option 010)	**Ultra High Oven** (Option 012 for 53132A only)
Temperature Stability (referenced to 25°C)		$< 5 \times 10^{-6}$	$< 2 \times 10^{-7}$	$< 2.5 \times 10^{-9}$	$< 2.5 \times 10^{-9}$
Aging Rate (after 30 days)	Per Day:		$< 4 \times 10^{-8}$	$< 5 \times 10^{-10}$	$< 1 \times 10^{-10}$
	Per Month:	$< 3 \times 10^{-7}$	$< 2 \times 10^{-7}$	$< 1.5 \times 10^{-8}$	$< 3 \times 10^{-9}$
	Per Year:				$< 2 \times 10^{-8}$
Turn-on stability vs. time (in 30 minutes)			$< 2 \times 10^{-7}$ referenced to 2 h	$< 5 \times 10^{-9}$ referenced to 24 h	$< 5 \times 10^{-9}$ referenced to 24 h
Calibration		Manual Adjust	Electronic	Electronic	Electronic

Note that power to the time base is maintained when the counter is placed in standby via the front panel switch. The internal fan will continue to operate when in standby to maintain long-term measurement reliability.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Instrument Inputs

Input Specifications

Channel 1 & 2 (53131A, 53132A)[1]
Channel 1 (53181A)

Frequency Range

dc Coupled	dc to 225 MHz
ac Coupled	1 MHz to 225 MHz (50 Ω) 30 Hz to 225 MHz (1 MΩ)
FM Tolerance	25%

Voltage Range and Sensitivity (Sinusoid)[2]

dc to 100 MHz	20 mVrms to ±5 V ac + dc
100 MHz to 200 MHz	30 mVrms to ±5 V ac + dc
200 MHz to 225 MHz	40 mVrms to ±5 V ac + dc (all specified at 75 mVrms with opt. rear connectors)[3]

Voltage Range and Sensitivity (Single-Shot Pulse)[2]

4.5 ns to 10 ns Pulse Width	100 mVpp to 10 Vpp (150 mVpp with optional rear connectors)[3]
>10 ns Pulse Width	50 mVpp to 10 Vpp (100 mVpp with optional rear connectors)[3]

Trigger Level[2]

Range	± 5.125 V
Accuracy	± (15 mV + 1% of trigger level)
Resolution	5 mV

Damage Level

50 Ω	5 Vrms
0 to 3.5 kHz, 1 MΩ	350 Vdc + ac pk
3.5 kHz to 100 kHz, 1 MΩ	350 Vdc + ac pk linearly derated to 5 Vrms
>100 kHz, 1 MΩ	5 Vrms

Input Characteristics

Channel 1 & 2 (53131A, 53132A)[1]
Channel 1 (53181A)

Impedance	1 MΩ or 50 Ω
1 MΩ Capacitance	30 pF
Coupling	ac or dc
Low-Pass Filter	100 kHz, switchable -20 dB at > 1 MHz
Input Sensitivity	Selectable between Low, Medium, or High (default). Low is approximately 2x High Sensitivity.
Trigger Slope	Positive or Negative

Auto Trigger Level

Range	0 to 100% in 10% steps
Frequency	> 100 Hz
Input Amplitude	> 100 mVpp (No amplitude modulation)

Attenuator

Voltage Range	x10
Trigger Range	x10

Input Specifications[4]

Channel 3 (53131A, 53132A)
Channel 2 (53181A)

Frequency Range

Option 015 (for 53181A only)	100 MHz to 1.5 GHz (see Opt. 030 for additional specs)
Option 030	100 MHz to 3 GHz
Option 050	200 MHz to 5 GHz
Option 124	200 MHz to 12.4 GHz

Power Range and Sensitivity (Sinusoid)

Option 030	100 MHz to 2.7 GHz: -27 dBm to +19 dBm 2.7 GHz to 3 GHz: -21 dBm to +13 dBm
Option 050	200 MHz to 5 GHz: -23 dBm to +13 dBm
Option 124	200 MHz to 12.4 GHz -23 dBm to +13 dBm

Damage Level

Option 030	5 Vrms
Option 050	+25 dBm
Option 124	+25 dBm

Characteristics

Impedance	50 Ω
Coupling	AC
VSWR	<2.5:1

External Arm Input Specifications[5]

Signal Input Range

TTL Compatible

Timing Restrictions

Pulse Width	> 50 ns
Transition Time	< 250 ns
Start-to-Stop Time	> 50 ns
Damage Level	10 Vrms

External Arm Input Characteristics[5]

Impedance	1 kΩ
Input Capacitance	17 pF
Start/Stop Slope	Positive or Negative

External Time Base Input Specifications

Voltage Range	200 mVrms to 10 Vrms
Damage Level	10 Vrms
Frequency	1 MHz, 5 MHz, and 10 MHz (53132A 10 MHz only)

Time Base Output Specifications

Output Frequency	10 MHz
Voltage	> 1 Vpp into 50 Ω (centered around 0 V)

1. Specifications and Characteristics for Channels 1 and 2 are identical for both common and separate configurations.
2. Values shown are for X1 attenuator setting. Multiply all values by 10 (nominal) when using the X10 attenuator setting.
3. When the 53131A or 53132A are ordered with the optional rear terminals (Opt. 060), the channel 1 and 2 inputs are active on both front and rear of the counter. When the 53181A is ordered with the optional rear terminal, the channel 1 input is active on both front and rear of the counter. For this condition, specifications indicated for the rear connections also apply to the front connections.
4. When optional additional channels are ordered with Opt. 060, refer to configuration table for Opt. 060 under ordering info on page 8. There is no degradation in specifications for this input, as applicable.
5. Available for all measurements except Peak Volts. External Arm is referred to as External Gate for some measurements.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

For Automatic or External Arming:
(and signals < 100 Hz using Timed Arming)

LSD Displayed: $\left(\frac{t_{res}}{Gate\ Time}\right) \times Frequency\ or\ Period$

RMS Resolution: $\left(\frac{\sqrt{t^2_{res} + 2 \times Trigger\ Error^2)}}{Gate\ Time}\right) \times Frequency\ or\ Period$

	53131A t_{res}	53132A t_{res}	53181A t_{res}
typical	650 ps	200 ps	650 ps

see graphs for worst case resolution performance

For Automatic Arming: $Gate\ Time = \frac{N}{Frequency}$

where N = 1 for standard channel Frequency < 1 MHz
4 for standard channel Frequency > 1 MHz
128 for optional channel

Systematic Uncertainty: $\left(\pm\ Time\ Base\ Error \pm \frac{t_{acc}}{Gate\ Time}\right) \times Frequency\ or\ Period$

	53131A t_{acc}	53132A t_{acc}	53181A t_{acc}
typical	350 ps	100 ps	350 ps
worst case	1.25 ns	500 ps	1.25 ns

Trigger: Default setting is Auto Trigger at 50%

For Time or Digits Arming:

LSD Displayed: $\left(\frac{2\sqrt{2} \times t_{res}}{Gate\ Time \times \sqrt{Number\ of\ Samples}} + \frac{t_{jitter}}{Gate\ Time}\right) \times Frequency\ or\ Period$

RMS Resolution (see graph 2): $\left(\frac{4 \times \sqrt{t^2_{res} + (2 \times Trigger\ Error^2)}}{Gate\ Time \times \sqrt{Number\ of\ Samples}} + \frac{t_{jitter}}{Gate\ Time}\right) \times Frequency\ or\ Period$

	53131A/181A		53132A	
	t_{res}	t_{jitter}	t_{res}	t_{jitter}
typical	500 ps	50 ps	225 ps	3 ps

see graphs for worst case resolution performance

Number of Samples = Gate Time x Frequency (Frequency < 200 kHz)
Gate Time x 200,000 (Frequency > 200 kHz)

Systematic Uncertainty: $\left(\pm\ Time\ Base\ Error \pm \frac{t_{acc}}{Gate\ Time}\right) \times Frequency\ or\ Period$

	53131A/181A	53132A
	t_{acc}	t_{acc}
typical	100 ps	10 ps
worst case	300 ps	100 ps

Trigger: Default setting is Auto Trigger at 50%

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Measurement Specifications

Frequency (53131A, 53132A, 53181A)

Channel 1 and 2 (53131A, 53132A)
Channel 1 (53181A)

Range	0.1 Hz to 225 MHz

Channel 3 (53131A, 53132A)
Channel 2 (53181A)

Option 015 (53181A only)	100 MHz to 1.5 GHz
Option 030	100 MHz to 3 GHz
Option 050	200 MHz to 5 GHz
Option 124	200 MHz to 12.4 GHz

(Period 2 or 3 selectable via GPIB only)

Period (53131A, 53132A, 53181A)

Channel 1 and 2 (53131A, 53132A)
Channel 1 (53181A)

Range	4.44 ns to 10 s

Channel 3 (53131A, 53132A)
Channel 2 (53181A)

Option 015 (53181A only)	0.66 ns to 10 ns
Option 030	0.33 ns to 10 ns
Option 050	0.2 ns to 5 ns
Option 124	80 ps to 5 ns

Frequency Ratio (53131A, 53132A, 53181A)

Measurement is specified over the full signal range of each input.

Results Range	10^{-10} to 10^{11}
"Auto" Gate Time	100 ms

Time Interval (53131A, 53132A)

Measurement is specified over the full signal ranges[6] of Channels 1 and 2.

Results Range	-1 ns to 10^5 s
LSD	500 ps (53131A)/150 ps (53132A)

Phase (53131A, 53132A)

Measurement is specified over the full signal range of Channels 1 and 2.

Results Range	-180° to +360°

Duty Cycle (53131A, 53132A)

Measurement is specified over the full signal range of Channel 1. However, both the positive and negative pulse widths must be greater than 4 ns.

Results Range	0 to 1 (e.g. 50% duty cycle would be displayed as .5)

Rise/Fall Time (53131A, 53132A)

Measurement is specified over the full signal ranges of Channel 1. The interval between the end of one edge and start of a similar edge must be greater than 4 ns.

Edge Selection	Positive or Negative
Trigger	Default setting is Auto Trigger at 10% and 90%
Results Range	5 ns to 10^5 s
LSD	500 ps (53131A)/150 ps (53132A)

Pulse Width (53131A, 53132A)

Measurement is specified over the full signal range of Channel 1. The width of the opposing pulse must be greater than 4 ns.

Pulse Selection	Positive or Negative
Trigger	Default setting is Auto Trigger at 50%
Results Range	5 ns to 10^5 s
LSD	500 ps (53131A)/150 ps (53132A)

Totalize (53131A, 53132A)

Measurement is specified over the full signal range of Channel 1.

Results Range	0 to 10^{15}
Resolution	± 1 count

Peak Volts (53131A, 53132A, 53181A)

Measurement is specified on Channels 1 and 2 for dc signals; or for ac signals of frequencies between 100 Hz and 30 MHz with peak-to-peak amplitude greater than 100 mV.

Results Range	-5.1 V to +5.1 V
Resolution	10 mV

Peak Volts Systematic Uncertainty

for ac signals: 25 mV + 10% of V
for dc signals: 25 mV + 2% of V

Use of the input attenuator multiplies all voltage specifications (input range, results range, resolution and systematic uncertainty) by a nominal factor of 10.

Gate Time

Auto Mode, or 1 ms to 1000 s

Measurement Throughput

GPIB ASCII	200 measurements/s (maximum)

Measurement Arming

Start Measurement	Free Run, Manual, or External
Stop Measurement	Continuous, Single, External, or Timed
Time Interval	100 µs to 10 s (53131A)
Delayed Arming	100 ns to 10 s (53132A)

Arming Modes

(Note that not all arming modes are available for every measurement function.)

5. Available for all measurements except Peak Volts. External Arm is referred to as External Gate for some measurements.
6. See Specifications for Pulse Width and Rise/Fall Time measurements for additional restrictions on signal timing characteristics

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Time Interval, Pulse Width, Rise/Fall Time (53131A and 53132A only):

RMS Resolution: $\sqrt{(t_{res})^2 + \text{Start Trigger Error}^2 + \text{Stop Trigger Error}^2}$

Systematic Uncertainty:

± (Time Base Error × Measurement) ± Trigger Level Timing Error ± 1.5 ns Differential Channel Error (53131A)
± (Time Base Error × Measurement) ± Trigger Level Timing Error ± 900 ps Differential Channel Error (53132A)
where t_{res} = 750 ps for the 53131A, 300 ps for the 53132A

Frequency Ratio: $\frac{Ch1}{Ch2}, \frac{Ch1}{Ch3}, \frac{Ch2}{Ch1}, \frac{Ch3}{Ch1}$ ***(53131A and 53132A)*** $\frac{Ch1}{Ch2}, \frac{Ch2}{Ch1}$ ***(53181A)***

LSD: Ratio $\frac{1}{2}$: $\frac{1}{Ch2\ Freq \times Gate\ Time}$ **Ratio $\frac{2}{1}$:** $\frac{Ch2\ Freq}{(Ch1\ Freq)^2 \times Gate\ Time}$

RMS Resolution: Ratio $\frac{1}{2}$: $\frac{2 \times \sqrt{1 + (Ch1\ Freq \times Ch2\ Trigger\ Error)^2}}{Ch2\ Freq \times Gate\ Time}$

Ratio $\frac{2}{1}$: $\frac{2 \times Ch2\ Freq \times \sqrt{1 + (Ch1\ Freq \times Ch2\ Trigger\ Error)^2}}{(Ch1\ Freq)^2 \times Gate\ Time}$

For measurements using Ch3, substitute Ch3 for Ch2 in these equations. To minimize relative phase measurement error, connect the higher frequency signal to channel 1.

Systematic Uncertainty: *± 2x resolution*

Phase (53131A and 53132A)

RMS Resolution: $\sqrt{((t_{res})^2 + (2 \times \text{Trigger Error}^2))} \times \left(1 + \left(\frac{Phase}{360°}\right)^2\right) \times Frequency \times 360°$

Systematic Uncertainty:

(±Trigger Level Timing Error ±1.5 ns Differential Channel Error) × Frequency × 360° (53131A)
(±Trigger Level Timing Error ±900 ps Differential Channel Error) × Frequency × 360° (53132A)

Duty Cycle (53131A and 53132A)

RMS Resolution: $\sqrt{((T_{res})^2 + (2 \text{ x Trigger Error}^2)) \text{ x } (1 + \text{Duty Cycle}^2) \times Frequency}$

t_{res}	53131A	53132A
	750 ps	300 ps

Auto Arming: Measurements are initiated immediately and acquired as fast as possible, using a minimum number of signal edges.

Timed Arming: The duration of the measurement is internally timed to a user-specified value (also known as the "gate time").

Digits Arming: Measurements are performed to the requested resolution (number of digits) through automatic selection of the acquisition time.

External Arming: An edge on the External Arm Input enables the start of each measurement. Auto Arming, Timed arming modes or another edge on the External Arm Input may be used to complete the measurement.

Time Interval Delayed Arming: For Time Interval measurements, the Stop Trigger condition is inhibited for a user-specified time following the Start Trigger. The 53132A offers advanced time interval arming capabilities including use of user specified time or Channel 2 events to delay both Start and Stop Triggers.

Measurement Limits

Limit Checking: The measurement value is checked against user-specified limits at the end of each measurement.

Display Modes: The measurement result may be displayed as either the traditional numeric value or graphically as an asterisk moving between two vertical bars.

Out-of-Limits Indications:

- The limits annunciator will light on the front panel display.
- The instrument will generate an SRQ if enabled via GPIB.
- The limits hardware signal provided via the RS-232 connector will go low for the duration of the out-of-limit condition.
- If the Analog Display mode is enabled, the asterisk appears outside the vertical bars, which define the upper and lower limits.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Fractional Time Base Error (see graph 3)

Time base error is the maximum fractional frequency variation of the time base due to aging or fluctuations in ambient temperature or line voltage:

$$\text{Time Base Error} = \left(\frac{\Delta f}{f}\,aging\ rate + \frac{\Delta f}{f}\,temperature + \frac{\Delta f}{f}\,line\ voltage \right)$$

Multiply this quantity by the measurement result to yield the absolute error for that measurement. Averaging measurements will not reduce (fractional) time base error. The counters exhibit negligible sensitivity to line voltage; consequently the line voltage term may be ignored.

Trigger Error

External source and input amplifier noise may advance or delay the trigger points that define the beginning and end of a measurement. The resulting timing uncertainty is a function of the slew rate of the signal and the amplitude of spurious noise spikes (relative to the input hysteresis band). The (rms) trigger error associated with a single trigger point is:

$$\text{Trigger Error} = \frac{\sqrt{(E_{input})^2 + (E_{signal})^2}}{Input\ Signal\ Slew\ Rate\ at\ Trigger\ Point}\ \text{(in seconds)}$$

where

E_{input} = RMS noise of the input amplifier: 1 mVrms (350 µVrms Typical). Note that the internal measurement algorithms significantly reduce the contribution of this term.

E_{signal} = RMS noise of the input signal over a 225 MHz bandwidth (100 kHz bandwidth when the low-pass filter is enabled). Note that the filter may substantially degrade the signal's slew rate at the input of the trigger comparator.

For two-trigger-point measurements (e.g. Rise Time, Pulse Width), the Trigger Errors will be referred to independently as Start Trigger Error and Stop Trigger Error.

Trigger Level Timing Error (see graph 6)

Trigger level timing error results from a deviation of the actual trigger level from the specified level. The magnitude of this error depends on resolution and accuracy of the trigger level circuit, input amplifier fidelity, input signal slew rate, and width of the input hysteresis band.

The following equations should be summed together to obtain the overall Trigger Level Timing Error. At the "High" sensitivity input setting, the hysteresis band can be assumed to be the sensitivity of the counter input (see page 2). Reduction of input sensitivity or use of the attenuator will increase the size of this band.

$$\text{Input Hysteresis Error:}\quad \frac{0.5 \times Hysteresis\ Band}{Input\ Signal\ Slew\ Rate\ at\ Start\ Trigger\ Point} - \frac{0.5 \times Hysteresis\ Band}{Input\ Signal\ Slew\ Rate\ at\ Stop\ Trigger\ Point}$$

$$\text{Trigger Level Setting Error:}\ \pm\ \frac{15\ mV \pm (1\% \times Start\ Trigger\ Level\ Setting)}{Input\ Signal\ Slew\ Rate\ at\ Start\ Trigger\ Point}\ \pm\ \frac{15\ mV \pm (1\% \times Stop\ Trigger\ Level\ Setting)}{Input\ Signal\ Slew\ Rate\ at\ Stop\ Trigger\ Point}$$

Differential Channel Error

The differential channel error term stated in several Systematic Uncertainty equations accounts for channel-to-channel mismatch and internal noise. This error can be substantially reduced by performing a TI calibration (accessible via the Utility Menu) in the temperature environment in which future measurements will be made.


Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Graph 1:
Agilent 53131A/181A–Worst Case RMS Resolution[7]
(Automatic or External Arming)


The graphs may also be used to compute errors for Period Measurements. To find the Period error (DP), calculate the frequency of the input signal (F = 1/P) and find the frequency error (DF) from the chart.

Then calculate the period error as:


$$\Delta P = \left(\frac{\Delta F}{F}\right) \times P$$

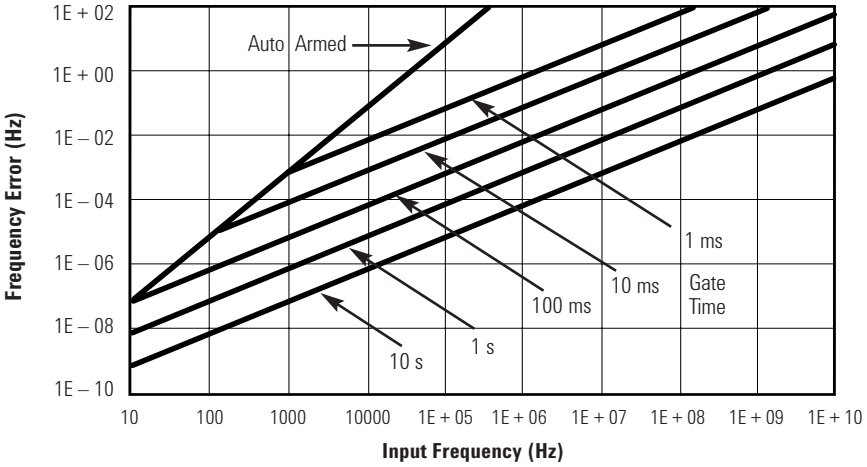

Graph 2:
Agilent 53131A/181A–Worst Case RMS Resolution[7]
(Time or Digits Arming)

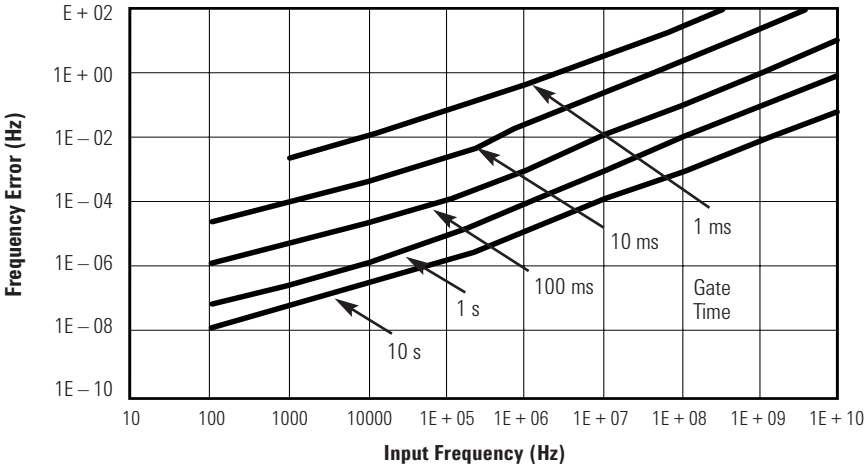

Graph 3:
Timebase Error

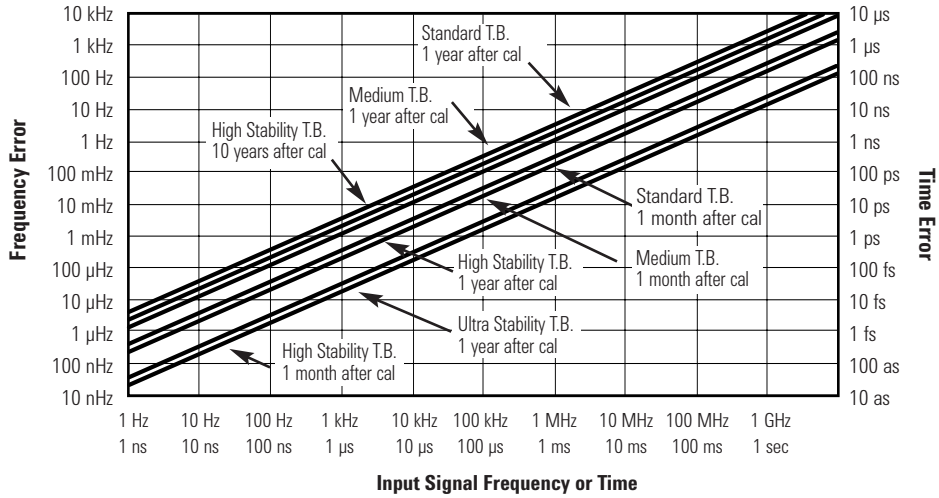

7. Graphs 1, 2, 4 and 5 do not reflect the effects of trigger error. To place an upper bound on the added effect of this error term, determine the frequency error from the appropriate graph and add a trigger error term as follows:

Time or Digit Arming


$$\text{Frequency Error} + \left(\frac{4 \times \sqrt{2} \times \text{Trigger Error}}{\text{Gate Time} \times \sqrt{\text{Number of Samples}}}\right) \times \text{Frequency or Period}$$

Automatic or External Arming


$$\text{Frequency Error} + \left(\frac{\sqrt{2} \times \text{Trigger Error}}{\text{Gate Time}}\right) \times \text{Frequency or Period}$$

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com


Graph 4:
Agilent 53132A–Worst Case RMS Resolution[7]
(Automatic or External Arming)

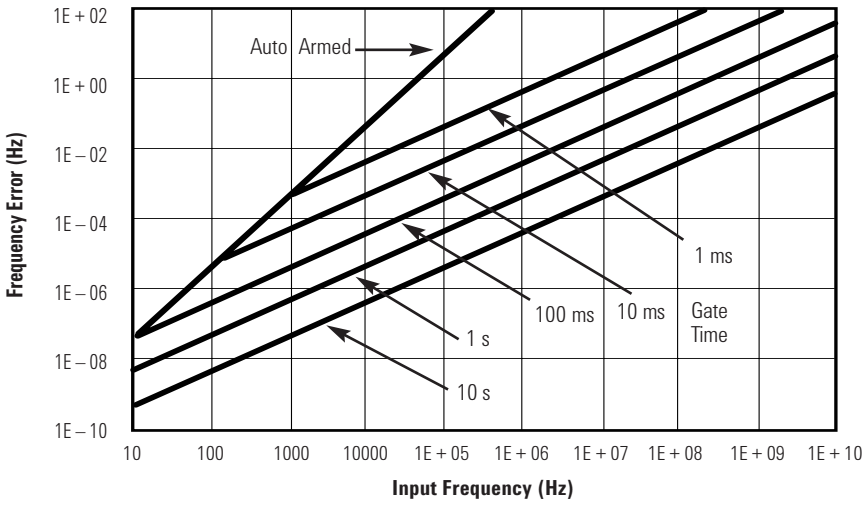

Graph 5:
Agilent 53132A–Worst Case RMS Resolution[7]
(Time or Digits Arming)

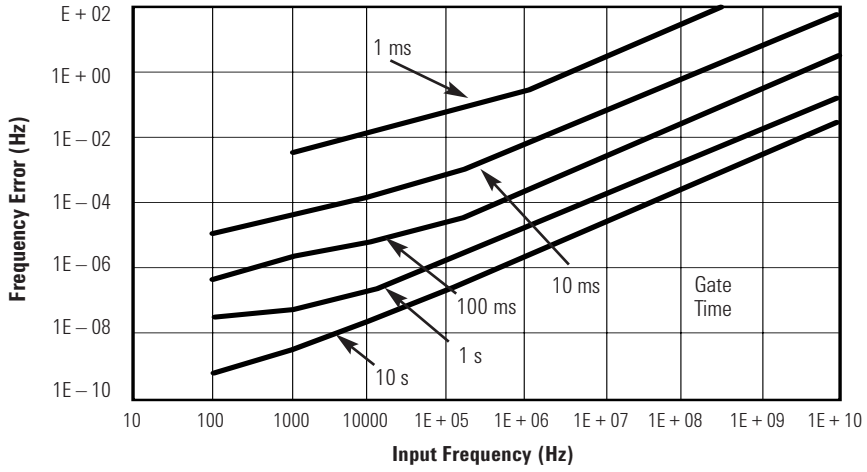

Graph 6:
Trigger Level Timing Error
(Level Setting Error and Input Hysteresis)

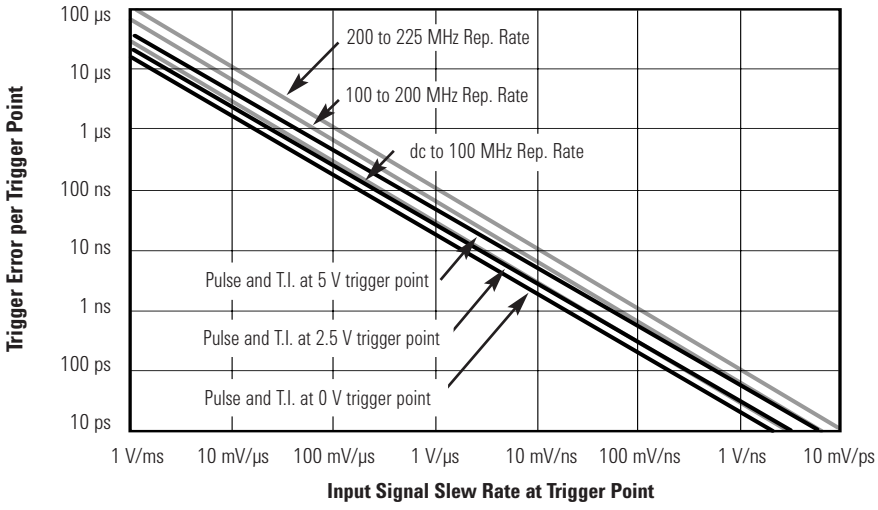

7. Graphs 1, 2, 4 and 5 do not reflect the effects of trigger error. To place an upper bound on the added effect of this error term, determine the frequency error from the appropriate graph and add a trigger error term as follows:

Time or Digit Arming

$$\text{Frequency Error} + \left(\frac{4 \times \sqrt{2} \times \text{Trigger Error}}{\text{Gate Time} \times \sqrt{\text{Number of Samples}}}\right) \times \text{Frequency or Period}$$

Automatic or External Arming

$$\text{Frequency Error} + \left(\frac{\sqrt{2} \times \text{Trigger Error}}{\text{Gate Time}}\right) \times \text{Frequency or Period}$$

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Measurement Statistics

Available Statistics

Mean, Minimum, Maximum, Standard Deviation

Number of Measurements 2 to 1,000,000.

Statistics may be collected on all measurements or on only those which are between the limit bands. When the Limits function is used in conjunction with Statistics, N (number of measurements) refers to the number of in-limit measurements. In general, measurement resolution will improve in proportion to N, up to the numerical processing limits of the instrument.

Measurements

Statistics may be collected for all measurements except Peak Volts and Totalize.

General Information

Save and Recall

Up to 20 complete instrument setups may be saved and recalled later. These setups are retained when power is removed from the counter.

Rack Dimensions (HxWxD)

88.5 mm x 212.6 mm x 348.3 mm

Weight

3.5 kg maximum

Warranty

1 year

Power Supply

100 to 120 VAC ± 10% -50, 60 or 400 Hz ± 10% 220 to 240 VAC ± 10% -50 or 60 Hz ± 10%

ac Line Selection

Automatic

Power Requirements

170 VA maximum (30 W typical)

Environment

0°C to 55°C operating
–40°C to 71°C storage

Remote Interface

GPIB (IEEE 488.1-1987, IEEE 488.2-1987)

Remote Programming Language

SCPI-1992.0 (Standard Commands for Programmable Instruments)

Safety

Designed in compliance with IEC-1010, UL-3111-1 (draft), CAN/CSA 1010.1

EMC

CISPR-11, EN50082-1, IEC 801-2, -3, -4

Radiated Immunity Testing

When the product is operated at maximum sensitivity (20 mVrms) and tested at 3 V/m according to IEC 801-3, external 100 to 200 MHz electric fields may cause frequency miscounts.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Ordering Information

53131A

10 digit/s, 500 ps Universal Counter

53132A

12 digit/s, 150 ps Universal Counter

53181A

10-digit/s RF Counter

Accessories Included

Each counter comes with IntuiLink software, standard timebase, power cord, operating, programming and service manuals.

Manual Options

(please specify one when ordering)

ABA	US English
ABD	German
ABE	Spanish
ABF	French
ABJ	Japanese
ABZ	Italian
AB0	Taiwan Chinese
AB1	Korean
AB2	Chinese

Other Options

Opt. 001	Medium-stability timebase
Opt. 010	High-stability timebase
Opt. 012	Ultra-high stability timebase (53132A only)
Opt. 015	1.5 GHz RF input Ch 2 for 53181A only
Opt. 030	3 GHz RF input Ch 3 (Ch 2 on 53181A)
Opt. 050	5 GHz RF input with type N connector Ch 3 (Ch 2 on 53181A)
Opt. 124	12.4 GHz RF input with type N connector Ch 3 (Ch 2 on 53181A)
Opt. 060	Rear-panel connectors*
Opt. 0B0	Delete manual set
Opt. A6J	ANSI Z540 compliant calibration
Opt. 1CM	Rack mount kit (P/N 5063-9240)**

***Opt 060 Configuration Table**

53131A/132A

Ch1 & Ch2	front & rear (in parallel)
Ch3	Opt. 030 rear only, front plugged
Ch3	Opt. 050/124 front only
Ch2	Opt. 050/124 front only


53181

Ch1	front & rear (in parallel)
Ch2	Opt. 015/030 rear only, front plugged
Ch2	Opt. 050/124 front only

** For racking two side-by-side, order both Lock-link Kit (P/N 5061-9694) and Flange Kit (P/N 5063-9212)

Accessories

34131A	Hard carrying case
34161A	Accessory pouch

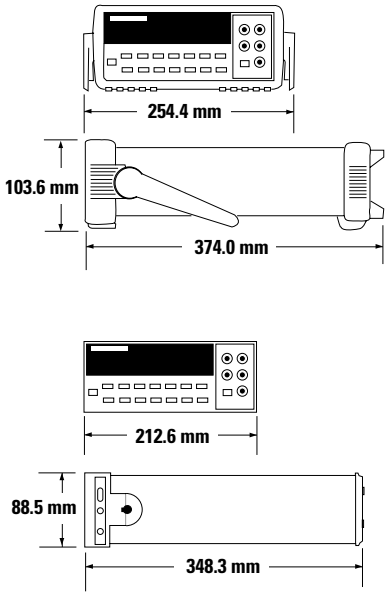

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Agilent Email Updates

www.agilent.com/find/emailupdates
Get the latest information on the products and applications you select.

Agilent Direct

www.agilent.com/find/quick
Quickly choose and use your test equipment solutions with confidence.

Agilent Open

www.agilent.com/find/open
Agilent Open simplifies the process of connecting and programming test systems to help engineers design, validate and manufacture electronic products. Agilent offers open connectivity for a broad range of system-ready instruments, open industry software, PC-standard I/O and global support, which are combined to more easily integrate test system development.

LXI is the US registered trademark of the LXI Consortium.

Remove all doubt

Our repair and calibration services will get your equipment back to you, performing like new, when promised. You will get full value out of your Agilent equipment throughout its lifetime. Your equipment will be serviced by Agilent-trained technicians using the latest factory calibration procedures, automated repair diagnostics and genuine parts. You will always have the utmost confidence in your measurements.

Agilent offers a wide range of additional expert test and measurement services for your equipment, including initial start-up assistance onsite education and training, as well as design, system integration, and project management.

For more information on repair and calibration services, go to

www.agilent.com/find/removealldoubt

www.agilent.com

For more information on Agilent Technologies' products, applications or services, please contact your local Agilent office. The complete list is available at:

www.agilent.com/find/contactus

Phone or Fax

United States:
(tel) 800 829 4444
(fax) 800 829 4433

Canada:
(tel) 877 894 4414
(fax) 800 746 4866

China:
(tel) 800 810 0189
(fax) 800 820 2816

Europe:
(tel) 31 20 547 2111

Japan:
(tel) (81) 426 56 7832
(fax) (81) 426 56 7840

Korea:
(tel) (080) 769 0800
(fax) (080) 769 0900

Latin America:
(tel) (305) 269 7500

Taiwan:
(tel) 0800 047 866
(fax) 0800 286 331

Other Asia Pacific Countries:
(tel) (65) 6375 8100
(fax) (65) 6755 0042
Email: tm_ap@agilent.com

Revised: 09/14/06

Product specifications and descriptions in this document subject to change without notice.

Microsoft® is a U.S. registered trademark of Microsoft Corporation

© Agilent Technologies, Inc. 2006
Printed in USA, November 27, 2006
5967-6039EN

Agilent Technologies

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Artisan Technology Group is an independent supplier of quality pre-owned equipment

Gold-standard solutions

Extend the life of your critical industrial, commercial, and military systems with our superior service and support.

We buy equipment

Planning to upgrade your current equipment? Have surplus equipment taking up shelf space? We'll give it a new home.

Learn more!

Visit us at **artisantg.com** for more info on price quotes, drivers, technical specifications, manuals, and documentation.

Artisan Scientific Corporation dba Artisan Technology Group is not an affiliate, representative, or authorized distributor for any manufacturer listed herein.

We're here to make your life easier. How can we help you today?

(217) 352-9330 | sales@artisantg.com | artisantg.com

ARTISAN® TECHNOLOGY GROUP