

ARTISAN®
TECHNOLOGY GROUP

Your **definitive** source for quality pre-owned equipment.

Artisan Technology Group
(217) 352-9330 | sales@artisantg.com | artisantg.com

Full-service, independent repair center
with experienced engineers and technicians on staff.

We buy your excess, underutilized, and idle equipment
along with credit for buybacks and trade-ins.

Custom engineering
so your equipment works exactly as you specify.

- Critical and expedited services
- In stock / Ready-to-ship
- Leasing / Rentals / Demos
- ITAR-certified secure asset solutions


Expert team | Trust guarantee | 100% satisfaction

All trademarks, brand names, and brands appearing herein are the property of their respective owners.

Visit our website - *Click HERE*

Quick Start Guide
MDA Scientific
Midas® Gas Detector
Pyrolyzer Module Option
(MIDAS-T-NP1)

Honeywell

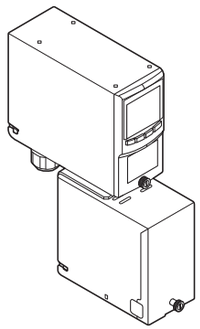

Introduction

The MIDAS-T-NP1 pyrolyzer option is installed under the standard Midas gas detector. The air sample is drawn through the pyrolyzer to the sensor cartridge. The pyrolyzer converts the target gas present in the air sample into hydrogen fluoride (HF) by means of pyrolysis. The HF can then be measured by the sensor and the concentration displayed as the equivalent reading in ppm of the target gas.

To maintain sensor accuracy when using the pyrolyzer, it is recommended to perform gas calibration every 6 months, and do not allow the ambient temperature at the point of installation to exceed 10-40°C (50–104°F) Operation above this temperature may require more frequent bump testing or calibration to confirm working specification. Because of the higher operating temperatures when using the pyrolyzer module, Honeywell Analytics strongly recommends that the ventilated Midas Top Cover (part number MIDAS-A-039) be used in all pyrolyzer applications.

Note: The Pyrolyzer module is serviceable only by trained personnel or by Honeywell Analytics' Service Center. Inappropriate handling can cause injury and device damage.

Gases that can be detected by the pyrolyzer are shown in this table.

Detectable Gases		
Cartridge Part No.	**Gas**	**Gas ID**
MIDAS-E-XHF, MIDAS-S-XHF	NF_3	01
	CH_3F	02
MIDAS-E-XCF, MIDAS-S-XCF	C_4F_6	01
	C_5F_8	02
	CH_2F_2	03

The unit's dimensions are shown in Figure 1.

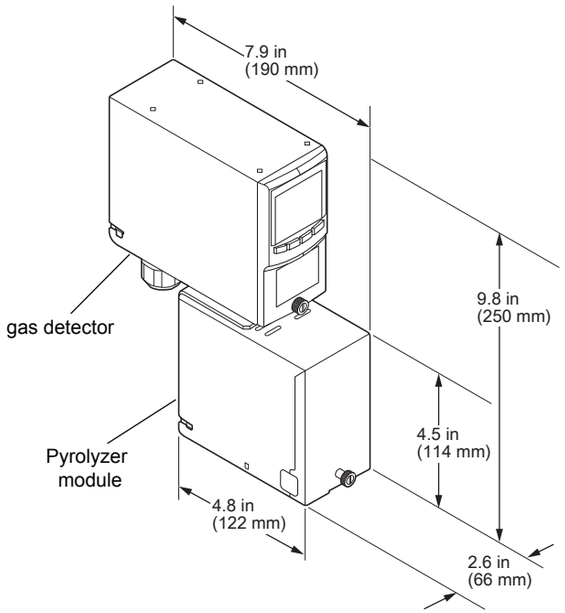


Figure 1: Dimensions

Fitting the Pyrolyzer Module

1. Disconnect power to the detector.
2. Unscrew the thumbscrew on the front panel.
3. Remove the cover by pulling it forward off the chassis (See Figure 2).

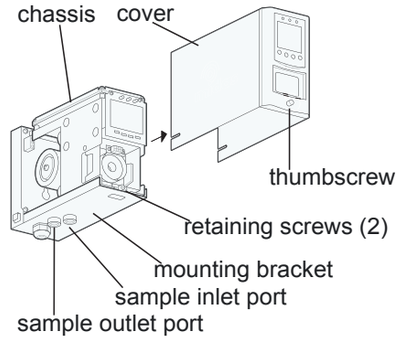


Figure 2: Removing the Midas cover

4. Unscrew the two retaining screws located at the bottom front of the chassis.
5. Pull the chassis forward to disconnect it from the mounting bracket assembly (see Figure 3).

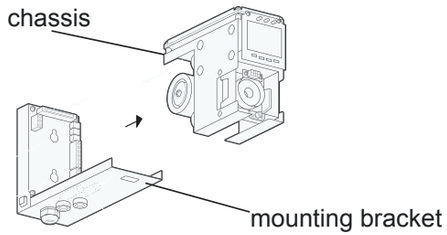


Figure 3: Removing the chassis

6. Thread the connector and wire harness from the pyrolyzer through the rectangular access in the bottom of the mounting bracket.
7. Secure the wires with a retention clip (if available).
8. Plug the connector into the socket (con5) at the bottom left of the terminal board.
9. Align the fitting at the top rear of the pyrolyzer with the sample inlet and outlet ports at the bottom of the mounting bracket.
10. Connect the pyrolyzer to the detector with the three provided mounting screws (see Figure 4).
11. The flow rate must be calibrated after installing or servicing the pyrolyzer. Refer to the Midas Technical Manual for the calibration procedure.

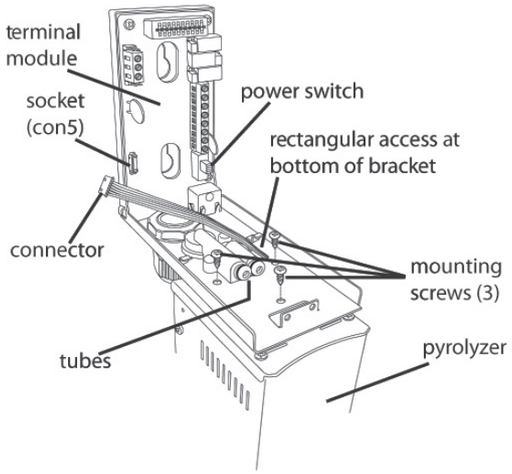


Figure 4: Attaching the pyrolyzer

Reassembling the Detector

1. Align:
   a. the PCB at the top rear of the chassis with the PCB connector at the top of the mounting bracket and
   b. the two tubes at the bottom rear of the chassis with the two tubes on the bottom of the mounting bracket.
2. Slide the chassis backward on the mounting bracket assembly so that the PCB, connector, and tubes engage fully. Push the chassis backward on the mounting bracket. CAUTION: The LCD is fragile. Do not apply pressure to its surface.
3. Tighten the retaining screws to secure the chassis to the mounting bracket.
4. Insert the sensor cartridge (see Figure 1) into the sensor cartridge chamber (Figure 5) and refer to the Sensor Cartridge Installation Quick Start Guide (MIDAS-A-021).

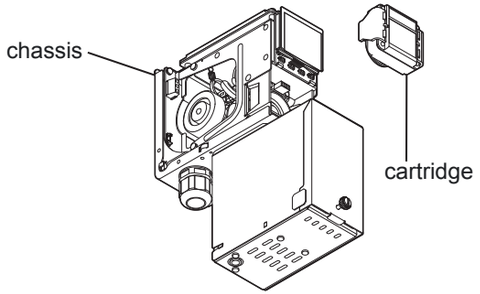


Figure 5: Reassembling the detector

5. Set the power switch to the “on” position.
6. Refit the ventilated top by aligning the slots on either side with the locating tabs on the mounting bracket assembly and pushing the cover horizontally until seated.

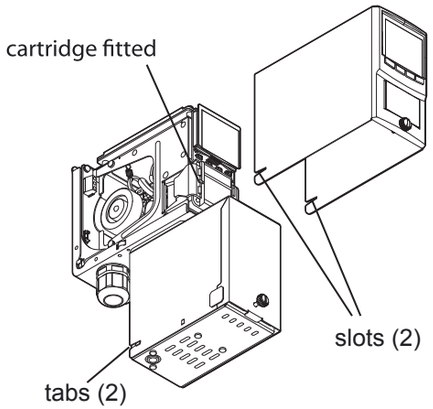


Figure 6: Refitting the top cover

7. Tighten the thumbscrew on the front panel.

Configuring the Detector

1. After completion of the startup sequence, press the “▲” button for a few seconds to select the setup menu.
2. Enter the passcode (if necessary).
3. Use the “▲” or “▼” buttons to select the setup menu “” icon. Press the “√” to accept.
4. Use the “▲” or “▼” buttons to select the set alarms “ ALm” submenu. Press “√” to accept.
5. The flashing gas ID code and the gas cylinder and alarms icon “” will appear.
6. Use the “▲” or “▼” buttons to change the gas ID number to that of the target gas . Press “√” to accept.
7. Continue to accept or change the rest of the alarm settings. For further details on these settings, refer to the Midas Operating Instructions (part number MIDAS-A-001).
8. Press “√” to update all changes (“UPdt” will be displayed).
9. Press “X” twice to return to normal operation.

Find out more
www.honeywellanalytics.com

Contact Honeywell Analytics:

Americas
Honeywell Analytics, Inc.
405 Barclay Blvd.
Lincolnshire, IL 60069
USA
Tel: +1 847 955 8200
Toll free: +1 800 538 0363
Fax: +1 847 955 8210
detectgas@Honeywell.com

Europe, Middle East, Africa
Life Safety Distribution GmbH
Javastrasse 2
8604 Hegnau
Switzerland
Tel: +41 (0)44 943 4300
Fax: +41 (0)44 943 4398
gasdetection@honeywell.com

Asia Pacific, India
Honeywell Analytics Asia Pacific, Co., Ltd.
7F SangAm IT Tower
434 Worldcup Buk-ro, Mapo-gu
Seoul 03922
South Korea
Tel: +82 (0)2 6909 0300
Fax: +82 (0)2 2025 0388
India Tel: +91 124 4752700
analytics.ap@honeywell.com

Honeywell

Part No. 3010M5020
Revision 1, August 2016
©2016 Honeywell Analytics

Artisan Technology Group is an independent supplier of quality pre-owned equipment

Gold-standard solutions

Extend the life of your critical industrial, commercial, and military systems with our superior service and support.

We buy equipment

Planning to upgrade your current equipment? Have surplus equipment taking up shelf space? We'll give it a new home.

Learn more!

Visit us at **artisantg.com** for more info on price quotes, drivers, technical specifications, manuals, and documentation.

Artisan Scientific Corporation dba Artisan Technology Group is not an affiliate, representative, or authorized distributor for any manufacturer listed herein.

We're here to make your life easier. How can we help you today?

(217) 352-9330 | sales@artisantg.com | artisantg.com

ARTISAN® TECHNOLOGY GROUP