ARTISAN®
TECHNOLOGY GROUP

Your **definitive** source for quality pre-owned equipment.

Artisan Technology Group
(217) 352-9330 | sales@artisantg.com | artisantg.com

Full-service, independent repair center
with experienced engineers and technicians on staff.

We buy your excess, underutilized, and idle equipment
along with credit for buybacks and trade-ins.

Custom engineering
so your equipment works exactly as you specify.

- Critical and expedited services
- In stock / Ready-to-ship
- Leasing / Rentals / Demos
- ITAR-certified secure asset solutions

Expert team | Trust guarantee | 100% satisfaction

All trademarks, brand names, and brands appearing herein are the property of their respective owners.

Find the *Instek SFG-2020* at our website: *Click HERE*

Synthesized Function Generator

SFG-2000/SFG-2100 Series

USER MANUAL

GW INSTEK PART NO. 82FG-21200MD



ISO-9001 CERTIFIED MANUFACTURER GW INSTEK

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

This manual contains proprietary information, which is protected by copyrights. All rights are reserved. No part of this manual may be photocopied, reproduced or translated to another language without prior written consent of Good Will company.

The information in this manual was correct at the time of printing. However, Good Will continues to improve products and reserves the rights to change specification, equipment, and maintenance procedures at any time without notice.

Good Will Instrument Co., Ltd.

No. 7-1, Jhongsing Rd., Tucheng City, Taipei County 236, Taiwan.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Table of Contents

SAFETY INSTRUCTIONS 5

Safety Symbols 5
Safety Guidelines 6

GETTING STARTED 9

Technical background 10
Lineup/Features 12
Front Panel 13
Rear Panel 19
Set Up 20
Operation Shortcuts 22
Default Setting Contents 24

SINE/SQUARE/TRIANGLE WAVE 25

Select the waveform 26
Set the Frequency 26
Set the Duty Cycle (Square Waveform) 28
Set Amplitude 29
Set Offset 30

TTL CMOS OUTPUT 31

Select the waveform 32
Set the Frequency 32
Set the Duty Cycle 33
Set Amplitude 34

SWEEP 35

AMPLITUDE MODULATION 37

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

FREQUENCY MODULATION 38

COUNTER INPUT 40

STORE/RECALL SETTING 42

APPLICATION EXAMPLES 44

Reference Signal for PLL System 44
Trouble-Shooting Signal Source 44
Transistor DC Bias Characteristics Test 45
Amplifier Over-Load Characteristic Test 46
Amplifier Transient Characteristics Test 46
Logic Circuit Test 48
Impedance Matching Network Test 48
Speaker Driver Test 49
Sweep for Speaker Test 50

FAQ 51

APPENDIX 52

Error Messages 52
Specification 53
Declaration of Conformity 55


INDEX 56

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

SAFETY INSTRUCTIONS

This chapter contains important safety instructions that you must follow when operating SFG-2000 series and when keeping it in storage. Read the following before any operation to insure your safety and to keep the best condition for SFG-2000 series.



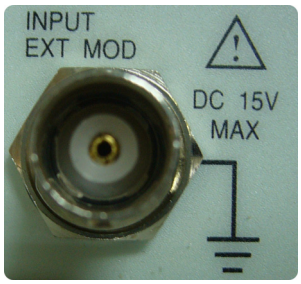

Safety Symbols

These safety symbols may appear in this manual or on SFG-2000 series.

WARNING	Warning: Identifies conditions or practices that could result in injury or loss of life.
CAUTION	Caution: Identifies conditions or practices that could result in damage to SFG-2000 series or to other properties.
	Attention Refer to the Manual
	Earth (ground) Terminal

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Safety Guidelines

General Guideline  CAUTION	• Do not place any heavy object on SFG-2000 series. • Avoid severe impacts or rough handling that leads to damaging SFG-2000 series. • Do not discharge static electricity to SFG-2000 series. • Use only mating connectors, not bare wires, for the terminals. • Do not block or obstruct cooling vent opening. • Do not perform measurements at power source and building installation site (Note below). • Do not disassemble SFG-2000 series unless you are qualified as service personnel. (Note) EN 61010-1:2001 specifies the measurement categories and their requirements as follows. SFG-2000 series falls under category II. • Measurement category IV is for measurement performed at the source of low-voltage installation. • Measurement category III is for measurement performed in the building installation. • Measurement category II is for measurement performed on the circuits directly connected to the low voltage installation.
Power Supply  WARNING	• Input voltage: 115/230V AC +10%, −15%, 50/60Hz • The power supply voltage should not fluctuate more than 10%. • Connect the protective grounding conductor of the power cord to earth ground, to avoid electrical shock.
Fuse  WARNING	• Fuse type: T0.125A/ 250V • Only service personnel are allowed to access internal fuse holders. • Replace the fuse with the specified type and rating only, for continued fire protection. • Disconnect the power cord before fuse replacement. • Make sure the cause of the fuse blowout is fixed before fuse replacement.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Cleaning SFG-2000 series	• Disconnect the power cord before cleaning. • Use a soft cloth dampened in a solution of mild detergent and water. Do not spray any liquid into SFG-2000 series. • Do not use chemicals or cleaners containing harsh materials such as benzene, toluene, xylene, and acetone.
Operation Environment	• Location: Indoor, no direct sunlight, dust free, almost non-conductive pollution (Note below) • Relative Humidity: < 80% • Altitude: < 2000m • Temperature: 0°C to 40°C (Note) EN 61010-1:2001 specifies the pollution degrees and their requirements as follows. SFG-2000 series falls under degree 2. Pollution refers to "addition of foreign matter, solid, liquid, or gaseous (ionized gases), that may produce a reduction of dielectric strength or surface resistivity". • Pollution degree 1: No pollution or only dry, non-conductive pollution occurs. The pollution has no influence. • Pollution degree 2: Normally only non-conductive pollution occurs. Occasionally, however, a temporary conductivity caused by condensation must be expected. • Pollution degree 3: Conductive pollution occurs, or dry, non-conductive pollution occurs which becomes conductive due to condensation which is expected. In such conditions, equipment is normally protected against exposure to direct sunlight, precipitation, and full wind pressure, but neither temperature nor humidity is controlled.
Storage Environment	• Location: Indoor • Relative Humidity: < 80% • Temperature: −10°C to 70°C

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Power cord for the United Kingdom


When using SFG-2000 series in the United Kingdom, make sure the power cord meets the following safety instructions.

NOTE: This lead / appliance must only be wired by competent persons

WARNING: THIS APPLIANCE MUST BE EARTHED

IMPORTANT: The wires in this lead are coloured in accordance with the following code:

Green/ Yellow:	Earth
Blue:	Neutral
Brown:	Live (Phase)



As the colours of the wires in main leads may not correspond with the colours marking identified in your plug/appliance, proceed as follows:

The wire which is coloured Green & Yellow must be connected to the Earth terminal marked with the letter E or by the earth symbol ⏚ or coloured Green or Green & Yellow.

The wire which is coloured Blue must be connected to the terminal which is marked with the letter N or coloured Blue or Black.

The wire which is coloured Brown must be connected to the terminal marked with the letter L or P or coloured Brown or Red.

If in doubt, consult the instructions provided with the equipment or contact the supplier.

This cable/appliance should be protected by a suitably rated and approved HBC mains fuse: refer to the rating information on the equipment and/or user instructions for details. As a guide, cable of 0.75mm2 should be protected by a 3A or 5A fuse. Larger conductors would normally require 13A types, depending on the connection method used.

Any moulded mains connector that requires removal /replacement must be destroyed by removal of any fuse & fuse carrier and disposed of immediately, as a plug with bared wires is hazardous if a engaged in live socket. Any re-wiring must be carried out in accordance with the information detailed on this label.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

GETTING STARTED

This chapter describes SFG-2000 series in a nutshell, including main features and front/rear/display introduction. Follow the Set Up section to properly install and power up SFG-2000 series.



SFG-2000 series overview	Technical background	10
	Series lineup	12
	Main features	12
Panel introduction	Front Panel	13
	Rear Panel	19
Setup	Tilt stand	20
	Power up	21
	Recall the default setting	21
	Functionality check	21
Quick reference	Operation Shortcuts	22
	Default Setting Contents	24

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Technical background

Traditional function generators

SFG-2000 series uses the latest Direct Digital Synthesis (DDS) technology to generate stable, high resolution output frequency. The DDS technology solves several problems encountered in traditional function generators, as follows.

Constant current circuit methodology

This analog function generating method uses a constant current source circuit built with discrete components such as capacitors and resistors. Temperature change inside the generator greatly affects the components characteristics which lead to output frequency change. The results are poor accuracy and stability.


DDS methodology

In DDS, the waveform data is contained in and generated from a memory. A clock controls the counter which points to the data address. The memory output is converted into analog signal by a digital to analog converter (DAC) followed by a low pass filter. The resolution is expressed as fs/2k where fs is the frequency and k is the control word, which contains more than 28bits. Because the frequency generation is referred to clock signal, this achieves much higher frequency stability and resolution than the traditional function generators.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Block diagram

DDS synthesizer consists of Phase accumulator (counter), lookout table data (ROM), Digital-to-analog converter (DAC), and Low-pass filter (LPF).

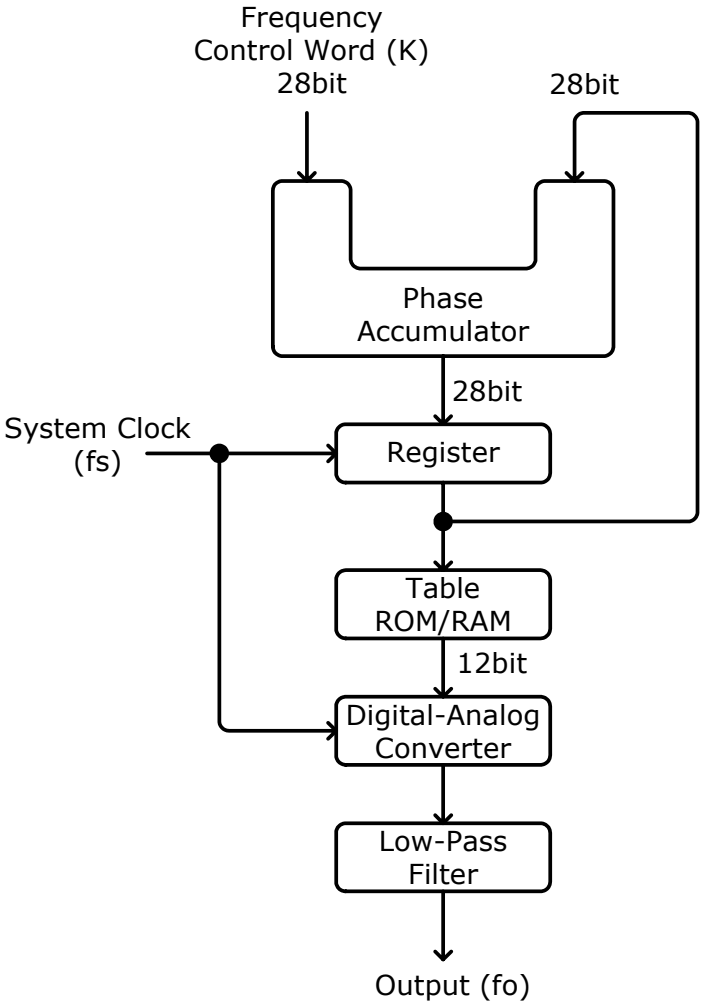

The phase accumulator adds the frequency control word K at every clock cycle fs. The accumulator output points to a location in the Table ROM/RAM. The DAC converts the digital data into an analog waveform. The LPF filters out the clock frequency to provide a pure waveform.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Lineup/Features

Series lineup

Lineup \ Features	Duty cycle	Offset	TTL/ CMOS	Sweep	AM/ FM	Counter
SFG-2004 (4MHz)	●	●	●	—	—	—
SFG-2007 (7MHz)	●	●	●	—	—	—
SFG-2010 (10MHz)	●	●	●	—	—	—
SFG-2020 (20MHz)	●	●	●	—	—	—
SFG-2104 (4MHz)	●	●	●	●	●	●
SFG-2107 (7MHz)	●	●	●	●	●	●
SFG-2110 (10MHz)	●	●	●	●	●	●
SFG-2120 (20MHz)	●	●	●	●	●	●


Main features

Performance	• High resolution using DDS and FPGA technology • High frequency accuracy: 20ppm • Low distortion: −55dBc • High resolution 100mHz maintained at full range
Features	• Wide output frequency range: 4, 7, 10, 20MHz • Various output waveforms: Sine, Square, and Triangle • TTL/CMOS output • Variable DC offset control • Output overload protection • Store/recall: 10 settings • Counter up to 150MHz high frequency (SFG-2100 series) • AM/FM with internal and external (SFG-2100 series) • Sweep mode with LINE and LOG (SFG-2100 series)
Input/Output Terminals	• Frequency output • TTL/CMOS output • Counter input (SFG-2100 series) • External modulation input (SFG-2100 series)


Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Front Panel

SFG-2100 series front panel

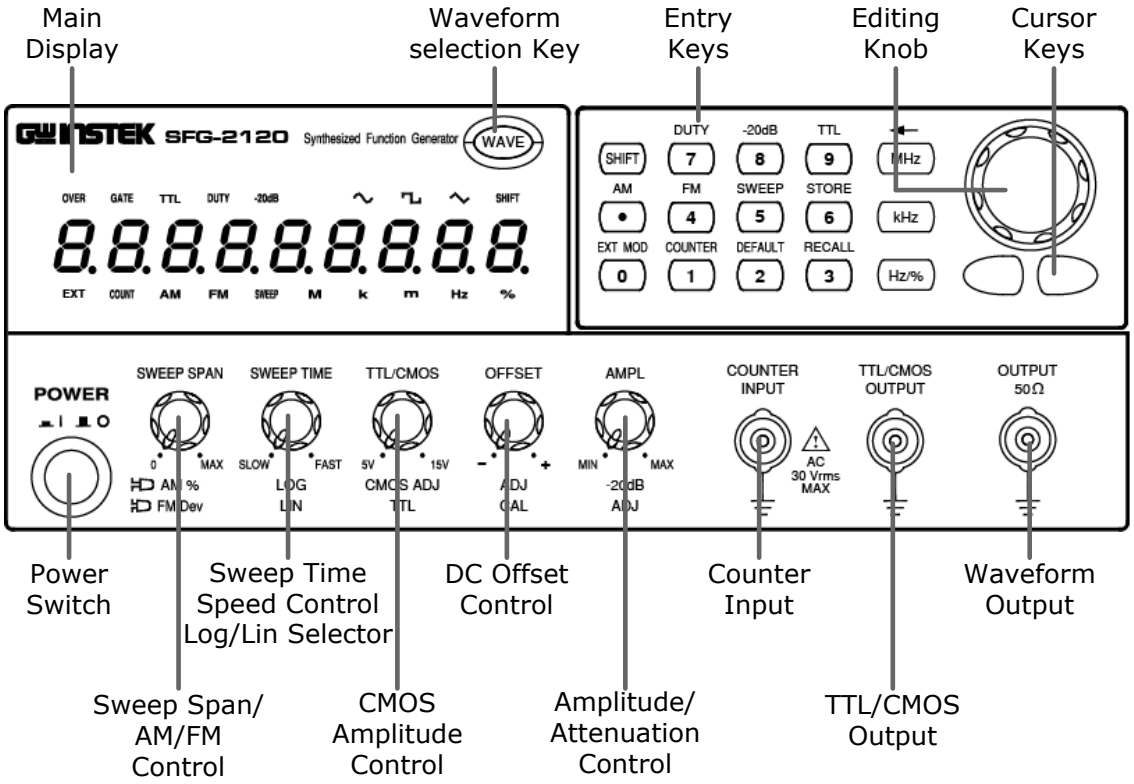

SFG-2000 series front panel

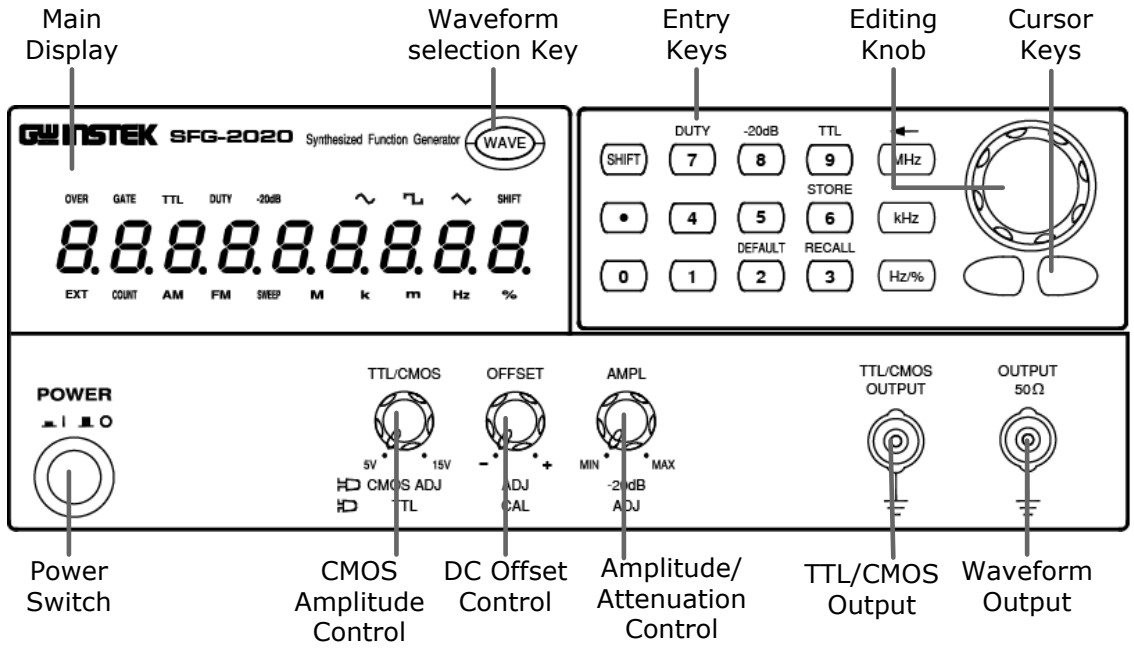

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Main display	 (7 segment)	Shows the waveform frequency, counter frequency, and duty cycle.
	OVER	For SFG-2100 series only. In the counter mode, indicates that the leftmost digit (100MHz) is hidden but contains a real number. For counter details, see page40.
	GATE	For SFG-2100 series only. In counter mode, indicates gate selection. For counter details, see page40.
	TTL	Indicates that the TTL or CMOS output is enabled. For TTL/CMOS details, see page31.
	DUTY	For square waveform only. Indicates that the duty cycle is being edited. For square waveform details, see page25.
	-20dB	Indicates that the waveform output is attenuated by −20dB. For attenuation details, see page29.
	SWEEP	For SFG-2100 series only. Indicates that the sweep mode is activated. For sweep details, see page35.
	FM AM	For SFG-2100 series only. Indicates that FM or AM mode is enabled. For modulation details, see page37 (AM) or page38(FM).
	COUNT	For SFG-2100 series only. Indicates that the counter mode is enabled. For counter details, see page40.
	EXT	For SFG-2100 series only. Indicates that the external modulation input is used. For details, see page37 (AM) or page39(FM).

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com



Indicates the waveform shape: Sine, Square, and Triangle. For details, see page26.

SHIFT — Indicates that the Shift key is pressed.

M k m Hz — Indicates the output frequency: MHz, kHz, or Hz.

% — Indicates the duty cycle unit. For duty cycle details, see page28.

Waveform selection key

WAVE — Selects the waveform shape: sine, square, and triangle. For details, see page26.

Entry keys

Enters frequency, duty cycle, and various parameters.

1 • 2 MHz — 1.2MHz

3 7 kHz — 37kHz

4 5 Hz/% — 45% (in duty cycle mode) 45Hz (in frequency mode)

SHIFT 7 (DUTY) — Enter duty cycle (page28).

SHIFT 8 (-20dB) — Attenuate the waveform output by −20dB (page29).

SHIFT 9 (TTL) — Enables TTL/CMOS output (page31).



SHIFT MHz (←) — Deletes previous entry (backspace).

SHIFT • (AM) — Selects Amplitude Modulation (page37).

SHIFT 4 (FM) — Selects Frequency Modulation (page38).


SHIFT 5 (SWEEP) — Selects sweep mode (page35).

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com


	STORE SHIFT 6	Stores the parameter setting (page42).
	RECALL SHIFT 3	Recalls the parameter setting (page42).
	DEFAULT SHIFT 2	Recalls the default parameter setting (page43).
	COUNTER SHIFT 1	Switches to counter mode (page40).
	EXT MOD SHIFT 0	Accepts external modulation signal (page37-AM) or (page38-FM).
Editing knob		Increases (right turn) or decreases (left turn) the frequency or duty cycle.
Cursor keys		Moves the editing point left or right in case of manual editing.
Waveform output	OUTPUT 50Ω 	Outputs sine, square, and triangle waveform. BNC terminal, 50Ω output impedance.
TTL/CMOS output	TTL/CMOS OUTPUT 	Outputs TTL or CMOS output waveform, BNC terminal. For TTL/CMOS mode details, see page31.
Counter input  Max AM 30Vrms	COUNTER INPUT 	Accepts signals for frequency counting. BNC, AC 30Vrms maximum. For counting mode details, see page40.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Amplitude/ Attenuation control




Sets the sine/square/triangle waveform amplitude. Turn left (decrease) or right (increase).




When pulled out, attenuates the sine/square/triangle waveform amplitude by −20dB. The −20dB display turns On.

For details, see page29.

DC offset control

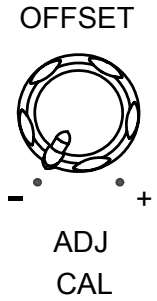



When pulled out, sets the DC offset level for sine/square/triangle waveform. Turn left (decrease) or right (increase). The range is −5V ~ +5V, in 50Ω load.

For details, see page30.


CMOS amplitude control



This knob becomes effective when the TTL/CMOS output is enabled (page31).



Selects TTL as output.




When pulled out, selects CMOS as output. Sets the CMOS output level. Turn left (decrease) or right (increase).

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Sweep speed control


Log/Linear sweep selector

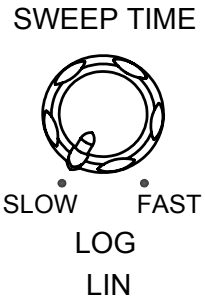

This knob is available in SFG-2100 series only. It becomes effective in sweep time mode.


Sets the sweep speed. Turn left (slow) or right (fast). The range is 1 ~ 30 seconds. For sweep details, see page35.

 Selects linear sweep.

 When pulled out, selects logarithmic sweep.

Sweep span control

AM/FM modulation control

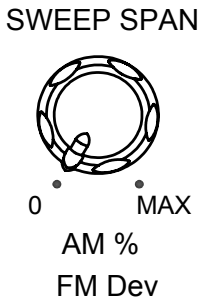


This knob is available in SFG-2100 series only. It becomes effective in sweep mode and AM/FM mode.


In Sweep mode: Sets the sweep span. Turn left (narrow) or right (wide). The range is 1 ~ 100. For sweep details, see page36.

In AM/FM mode:

 Sets the FM deviation (page38). Turn left (decrease) or right (increase). The range is over −50kHz ~ +50kHz, centered at 1MHz.

 When pulled out, sets the AM depth (page37). Turn left (shallow) or right (deep). The range is 0 ~ 100%.


Power switch



Turns the main power On/Off. For power up sequence, see page20.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Rear Panel

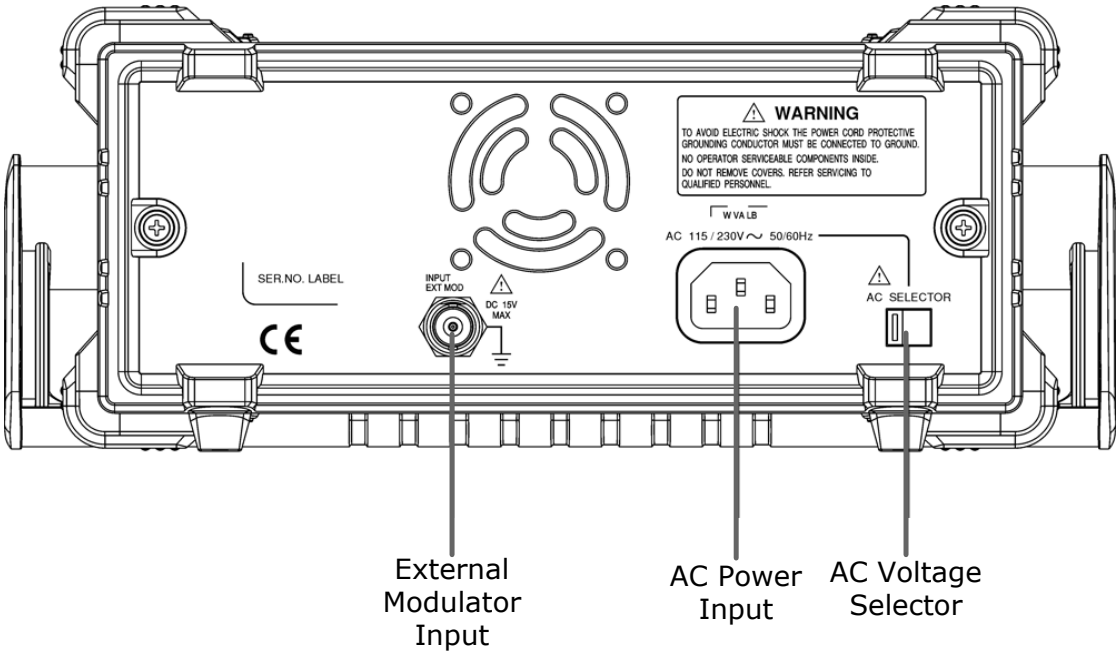


External Modulator Input	Accepts the modulation signal from external device. BNC male connector, 10Vp-p maximum. SFG automatically switches the modulation signal from internal to external. For modulation details, see page37 (AM) or page38(FM).
AC Power Input	Accepts the AC power cord. 115 or 230V, 50/60Hz.
AC Voltage Selector	Selects 115V or 230V for power source. AC 100/110/120V → select 115V. AC 220/230/240V → select 230V. ⚠ Improper selection might lead to internal fuse blowout.


Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Set Up


Tilt stand

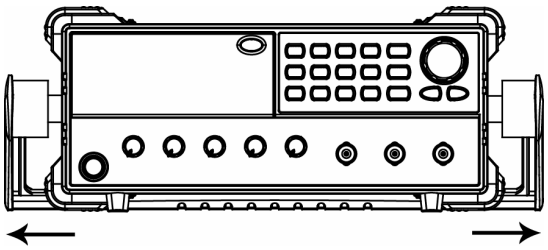


Pull out the handle sideways and rotate it.

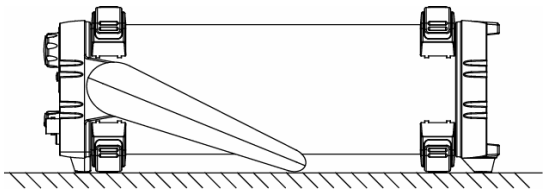

Place SFG horizontally,

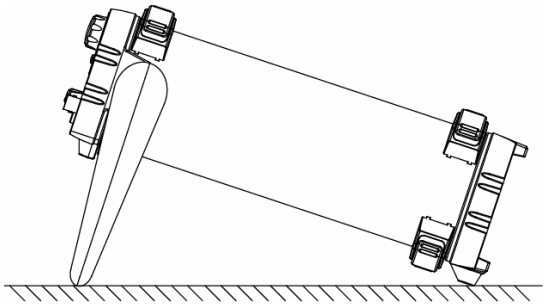

Or tilt stand.

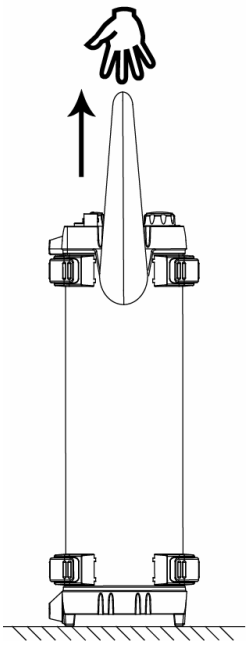

Place the handle vertically for hand carry.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com


Power up




1. Select the AC voltage on the rear panel accordingly.
   AC 100/110/120V→select 115V.
   AC 220/230/240V→select 230V.



2. Connect the power cord.



3. Push and turn On the main power switch on the front panel.



4. The display shows model name and the last setup. Example: SFG-2110, 500Hz triangle wave in sweep mode and −20dB attenuation enabled




Recall the default setting

Press DEFAULT SHIFT 2 to recall the default setup. SFG shows the message "done", and outputs 10kHz sine wave.



Functionality check

Connect SFG output to measurement device such as oscilloscope and check the waveform characteristics.

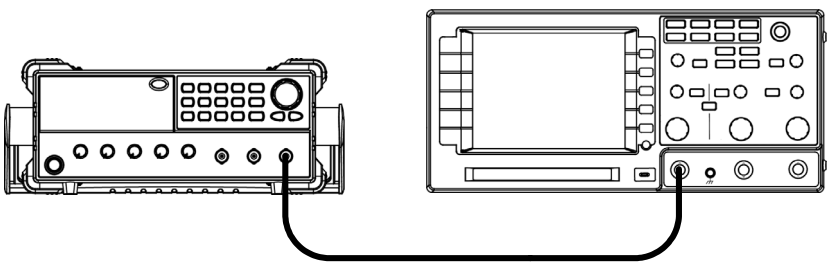









Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Operation Shortcuts

Here are the collections of operation example shortcuts.

Sine wave 250Hz, −20dB amplitude OUTPUT 50Ω	1. Press Wave key and select Sine	WAVE
	2. Press 2 + 5 + 0 + Hz/% key	2 5 0 Hz/%
	3. Press Shift + 8 key (−20dB) ...Or pull Amplitude knob	SHIFT 8 (-20dB) -20dB or AMPL ADJ
Triangle wave 8kHz, +2V Offset OUTPUT 50Ω	1. Press Wave key and select Triangle	WAVE
	2. Press 8 + kHz key	8 kHz
	3. Pull Offset knob (ADJ) and Rotate	OFFSET ADJ
Square Wave 1MHz, 45% duty OUTPUT 50Ω	1. Press Wave key and select Square	WAVE
	2. Press 1 + MHz key	1 MHz
	3. Press Shift + 7 key (Duty)	SHIFT 7 (DUTY) DUTY
	4. Press 4 + 5 + Hz/% key ...Or Rotate the Scroll knob	4 5 Hz/% or
TTL Output 10kHz TTL/CMOS OUTPUT	1. Press Shift + 9 key (TTL)	SHIFT 9 (TTL) TTL
	2. Press 1 + 0 + kHz key	1 0 kHz
	3. Press TTL/CMOS knob (TTL)	TTL/CMOS (TTL)
CMOS Out 10kHz, 10Vpp TTL/CMOS OUTPUT	1. Press Shift + 9 key (TTL)	SHIFT 9 (TTL) TTL
	2. Press 1 + 0 + kHz key	1 0 kHz
	3. Pull TTL/CMOS knob (CMOS) and rotate	TTL/CMOS (CMOS)

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Linear Sweep, 1kHz start, Sine wave 250Hz OUTPUT 50Ω 	1. Press Wave key and select Sine	
	2. Press 2 + 5 + 0 + Hz/% key	
	3. Press Shift + 5 key (Sweep)	
	4. Press SWEEP TIME knob (LIN) and rotate	SWEEP TIME LIN 
	5. Press SWEEP SPAN knob and rotate	SWEEP SPAN 
Log Sweep, 10kHz start, Triangle wave 8kHz OUTPUT 50Ω 	1. Press Wave key and select Triangle	
	2. Press 8 + kHz key	
	3. Press Shift + 5 key (Sweep)	
	4. Pull SWEEP TIME knob (LOG) and rotate	SWEEP TIME LOG 
	5. Press SWEEP SPAN knob and rotate	SWEEP SPAN 
AM, Internal, 50% modulation, sine wave 10kHz OUTPUT 50Ω 	1. Press Wave key and select Sine	
	2. Press 1 + 0 + kHz key	
	3. Press Shift + .(dot) key (AM)	
	4. Pull SWEEP SPAN knob (AM %) and rotate	SWEEP SPAN 
FM, External, 50% deviation, sine wave 1MHz OUTPUT 50Ω 	1. Press Wave key and select Sine	
	2. Press 1 + MHz key	
	3. Input external modulation signal (EXT sign appears)	
	4. Press Shift + 4 key (FM)	
	5. Push SWEEP SPAN knob (FM Dev) and rotate	SWEEP SPAN (FM Dev) 

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Counter input, sine wave 1MHz COUNTER INPUT 	1. Press Shift + 1 (Counter)	SHIFT COUNTER 1 COUNT
	2. The Gate sign flashes when counted	GATE
Store the setting to memory No.1	1. Press Shift + 6 (Store)	SHIFT STORE 6
	2. The "Store" sign appears	StorE 0
	3. Enter the memory number (1 ~ 10)	StorE 1
	4. The "done" sign appears	donE
Recall the setting from memory No.1	1. Press Shift + 3 (Recall)	SHIFT RECALL 3
	2. The "Recall" sign appears	rEcALL 0
	3. Enter the memory number (1 ~ 10)	rEcALL 1
	4. The "done" sign appears	donE

Default Setting Contents

Recall default settings

SHIFT DEFAULT 2

Press the shift key, then 2 to recall the default setting. The "done" message appears, followed by display update.

donE
10.0000 k Hz

Wave type	Sine wave
Frequency	10.0000kHz
TTL/CMOS	Disabled
−20dB	Disabled
Modulation	Disabled
Sweep mode	Disabled

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

SINE/SQUARE/TRIANGLE WAVE



Select waveform	Select the waveform	26
Set frequency	Enter frequency	26
	Edit frequnency	27
Set duty cycle (for square wave)	Enter duty cycle	28
	Edit duty cycle	28
Set amplitude	Normal output	29
	Attenuate by −20dB	29
Set offset	Activate offset	30
	Adjust offset	30
	Limitation	30

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Select the waveform

Sine / Square / Triangle

Press WAVE key repeatedly. The corresponding icon appears on the display.



Sine waveform.




Square waveform.



Triangle waveform.

OUTPUT 50Ω

The waveform comes out from the main terminal.



10Vp-p maximum (50Ω load)

20Vp-p maximum (no load)

Set the Frequency

Enter frequency

Enter the waveform frequency using the numerical keys.

1 • 2 MHz — 1.2MHz

3 7 kHz — 37kHz

4 5 Hz/% — 45Hz

SHIFT MHz — Delete a number (backspace)

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Triangle waveform frequency is limited to maximum 1MHz. When the input exceeds it, the following message (Freq-Err2) appears and forces the frequency to 1MHz.




For full error message list, see page52.

Edit frequency





Left cursor key moves the active cursor left.

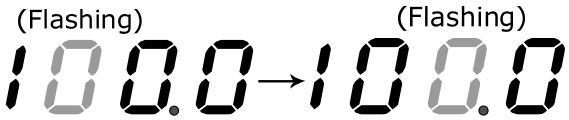





Right cursor key moves the active cursor right.

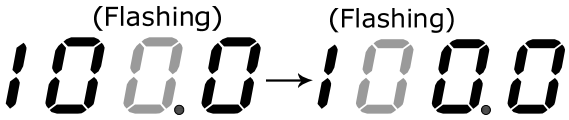




Turn the editing knob left to decrease the frequency.

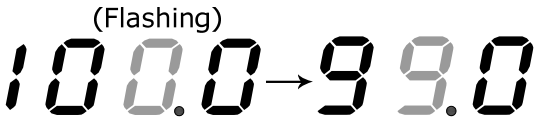



Turn the editing knob right to increase the frequency.



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Set the Duty Cycle (Square Waveform)

The duty cycle setting is not available in sine/triangle waveform.

Enter duty cycle



Press the Shift key, then 7 to enter duty cycle editing mode. The duty sign appears on the display.




The default value is 50%.

The settable range is 20% ~ 80%, 2Hz ~ 1MHz.




Use numerical keys to enter value.
Example: 45%



Delete a number (backspace)

Edit duty cycle




The editing knob changes the value, and the cursor keys moves the active digit (same as entering frequency).

When inactive for 5 seconds, the display automatically goes back to previous mode (frequency view).

Setting duty cycle (press 

) is not available when sine or triangle waveform is activated. The following message appears.




For full error message list, see page52.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Set Amplitude

Normal output

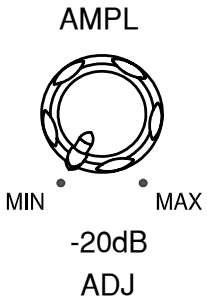


Turn the Amplitude knob right (increase) or left (decrease).

The range is 10Vpp for 50Ω load.


Attenuate by −20dB

Sine/square/triangle waveform can be attenuated by −20dB, in two ways: −40dB altogether.



Method1

Pull out the Amplitude knob. The output amplitude is attenuated by −20dB (no display sign).





Method2


Press the shift key, then 8. The output amplitude is attenuated by −20dB. The −20dB sign appears on the display.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com


Set Offset

Activate offset

SFG can add or delete offset to the sine/square/triangle waveform, thus changing the waveform vertical position. Use the OFFSET knob.




Pushed: Offset Off



Pulled: Offset On

Adjust offset

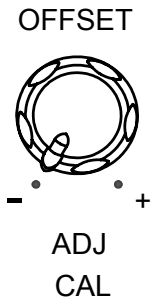

Turn the knob right (higher position) or left (lower position).

The range is −5V ~ +5V for 50Ω load.

Limitation


Note that the output amplitude, including the offset, is still limited to:

−5 ~ +5V (50Ω load)


−10 ~ +10V (no load)

Therefore excessive offset leads to peak clip as below.

Positive peak clip (50Ω)

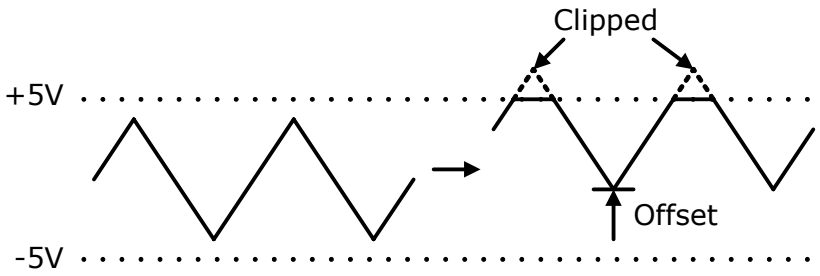

Negative peak clip (50Ω)

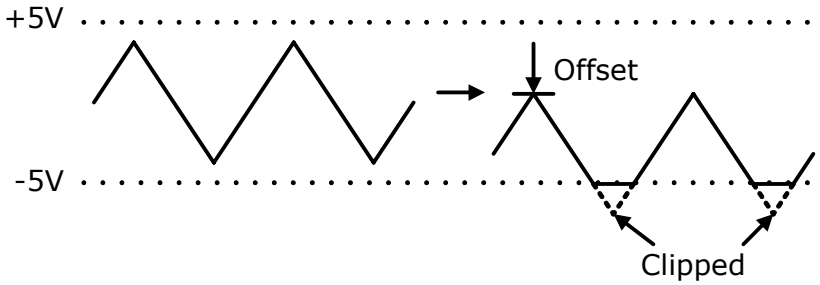

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

TTL CMOS OUTPUT




Select waveform	Select the waveform	32
Set frequency	Enter frequency	32
	Edit frequency	33
Set duty cycle	Enter duty cycle	33
	Edit duty cycle	34
Set amplitude	Set Amplitude	34

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Select the waveform

TTL/CMOS




Press Shift key, then 9. The TTL sign appears on the display.




The TTL/CMOS output is always On when the square wave is activated.




Push/pull the TTL/CMOS knob to select the waveform.



Pushed: TTL is selected as output.



Pulled: CMOS is selected as output.



The waveform comes out from the TTL/CMOS terminal.

TTL: ≥3Vp-p (fixed)

CMOS: 4V±1Vp-p ~ 15±1Vp-p

Set the Frequency

Enter frequency

Enter the waveform frequency using the numerical keys.




1.2MHz



37kHz



45Hz




Delete a number (backspace)

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Edit frequency





Left cursor key moves the active cursor left.

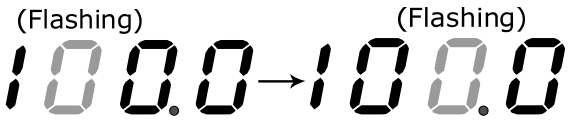





Right cursor key moves the active cursor right.

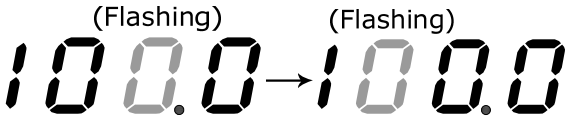




Turn the editing knob left to decrease the frequency.

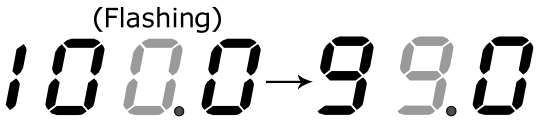




Turn the editing knob right to increase the frequency.



Set the Duty Cycle

Enter duty cycle



Press the Shift key, then 7 to enter duty cycle editing mode. The duty sign appears on the display.




The default value is 50%.

The settable range is 20% ~ 80%, 2Hz ~ 1MHz.




Use the numerical keys to enter value. Example: 45%



Delete a number (backspace)

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Edit duty cycle




The editing knob changes the value, and the cursor keys moves the active digit (same as entering frequency).


When inactive for 5 seconds, the display automatically goes back to previous mode (frequency view).


Set Amplitude

CMOS waveform

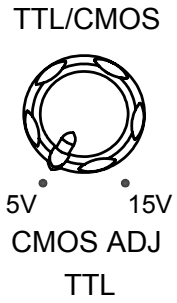

Use the TTL/CMOS knob.

 Pushed: selects TTL output with fixed amplitude, min. 3Vp-p.

 Pulled: selects CMOS output, amplitude range 4V±1Vp-p ~ 15±0.5Vp-p.

Turn the knob right (increase amplitude) or left (decrease amplitude).

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

SWEEP


SFG can add sweep to the waveform output, a convenient tool for measuring the frequency response of the DUT.



- Sweep function applies only to SFG-2100 series.
- Sweep and Modulation (page37) cannot be used together.

Activate sweep

1. Output the waveform. Sine/Triangle/Square (page25) or TTL/CMOS (page31).
2. Press the Shift key, then 5 (Sweep).




3. Sweep is activated and the sign appears on the display.

SWEEP

When the sweep is activated, the duty cycle of Square/TTL/CMOS wave is fixed to 50%.

Select Log/Lin Sweep

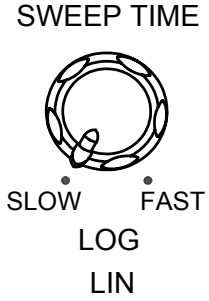

Logarithmic Sweep:

Pull the SWEEP TIME knob.

Linear Sweep:


Push the SWEEP TIME knob.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Set Sweep Time

Sweep time sets the time it takes for a single sweep from the start frequency to the end frequency.

Rotate the SWEEP TIME knob, right (fast) or left (slow).



Range 1 ~ 30 seconds


Note: If the sweep time becomes too long, the stop frequency might reach the rating (4, 7, 10, or 20MHz). In this case, the frequency stays at the rating to the end.

Set Sweep Span

Sweep span sets the frequency width of the sweep.

The current output frequency becomes the start frequency.

Rotate the SWEEP SPAN knob, right (wide) or left (narrow).



Range 1 ~ 100 frequency ratio

Note: In order to get the maximum span (frequency ratio), set the sweep time to a sufficient length (not too short).

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com


AMPLITUDE MODULATION



- AM applies only to SFG-2100 series.
- Modulation and Sweep (page35) cannot be used together.

Activate AM

1. Output the waveform, Sine/Triangle/Square (page25).
2. Press the Shift key, then Dot (AM). AM is activated and the sign appears on the display.




Set AM depth



1. Pull the SWEEP SPAN knob (AM %).
2. Turn the knob left (shallow) or right (deep).

Range	0 ~ 100%

Use external modulating signal



SFG-2000 series uses an internal 400Hz sine wave as the default modulating signal.

1. Connect the modulating signal to the rear panel terminal.
2. Press the Shift key, then 0 (EXT MOD). External modulation is activated.



Frequency Range	DC ~ 1MHz

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

FREQUENCY MODULATION



- FM applies only to SFG-2100 series.
- Modulation and Sweep (page35) cannot be used together.

Activate FM


1. Output the waveform. Sine/Triangle/Square (page25) or TTL/CMOS (page31).
2. Press the Shift key, then 4 (FM). FM is activated and the sign appears on the display.



When FM is activated, the duty cycle of Square/TTL/CMOS wave is fixed to 50%.

Set FM deviation

The output frequency becomes the Center Frequency.

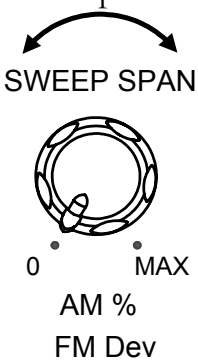

1. Push the SWEEP SPAN knob (FM Dev).



2. Turn the knob left (shallow) or right (deep).


Deviation Range	0 ~ ±50kHz, centered at 1MHz

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

When the deviation is added to the center frequency, the result must be smaller than the rating frequency.

Center Frequency + Deviation ≤ Rating**(4,7,10,20MHz)**

When this rule is violated, the "Freq-Err3" error message appears and the FM setting will be cancelled.




For more error message details, see page52.

Center frequency (=Output frequency) must be set within this range.

SFG-2104	300kHz ~ 3.7MHz
SFG-2107	300kHz ~ 6.7MHz
SFG-2110	300kHz ~ 9.7MHz
SFG-2120	300kHz ~ 19.7MHz

Use external modulating signal



SFG-2000 series uses an internal 400Hz sine wave as the default modulating signal.

1. Connect the modulating signal to the rear panel terminal.
2. Press the Shift key, then 0 (EXT MOD). External modulation is activated.



Frequency Range	1kHz (fixed)


Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

COUNTER INPUT



Counter input applies only to SFG-2100 series.

Activate counter




1. Connect the signal input to the Counter input terminal. Press Shift key, then 1 (Counter).



2. EXT and COUNT sign appear on the display.



3. The display shows the input signal frequency.

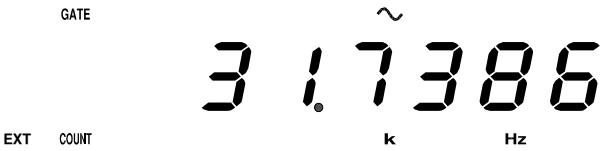

4. The GATE sign flashes when the gate condition is met.




Range	0 ~ 150MHz
Resolution	100nHz for 1Hz input, 0.1Hz for 100MHz input

Set the gate time

Gate time sets the display update rate and counter resolution. These two parameters are in trade-off.

Short gate time = faster update, coarse resolution

Long gate time = slower update, fine resolution



To change the gate time, turn the editing knob right (increase) or left (decrease).

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Gate time / Resolution table

The following table shows the relationship between counter frequency, gate time, resolution, and display.

Input	Gate time	Resolution	Display
1Hz	0.01s	100μHz	1.0000Hz
	0.1s	10μHz	1.00000Hz
	1s	1μHz	1.000000Hz
	10s	100nHz	1.0000000Hz
10Hz	0.01s	100μHz	10.0000Hz
	0.1s	10μHz	10.00000Hz
	1s	1μHz	10.000000Hz
	10s	100nHz	10.0000000Hz
100Hz	0.01s	1mHz	100.000Hz
	0.1s	100μHz	100.0000Hz
	1s	10μHz	100.00000Hz
	10s	1μHz	100.000000Hz
1kHz	0.01s	10mHz	1.00000kHz
	0.1s	1mHz	1.000000kHz
	1s	100μHz	1.0000000kHz
	10s	10μHz	1.00000000kHz
1MHz	0.01s	10Hz	1.00000MHz
	0.1s	1Hz	1.000000MHz
	1s	100mHz	1.0000000MHz
	10s	10mHz	1.00000000MHz
10MHz	0.01s	100Hz	10.0000MHz
	0.1s	10Hz	10.00000MHz
	1s	1Hz	10.000000MHz
	10s	100mHz	10.0000000MHz
100MHz	0.01s	100Hz	100.0000MHz
	0.1s	10Hz	100.00000MHz
	1s	1Hz	100.000000MHz
	10s	100mHz	00.0000000MHz*

Over sign

* The OVER sign shows that the 100MHz digit contains a real number but hidden from the display. It turns On under the following condition.

- Input frequency: ≥100MHz
- Gate Time: 10s

To view the 100MHz digit, switch to smaller gate time such as 1s or 0.1s.



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

STORE/RECALL SETTING



Store the panel setting



Press the Shift key, then 6 to store the current panel setting to internal memories.
Memory range: 0 ~ 9 (10 set)

The "Store 0" sign appears.



Enter the memory number, 0 ~ 9. (for example, 1)



The "done" sign appears.




Recall the panel setting




Press the Shift key, then 3 to recall a panel setting stored in internal memories.
Memory range: 0 ~ 9 (10 set)

The "recall 0" sign appears.



Enter the memory number, 0 ~ 9. (for example, 1)



The "done" sign appears and the panel setting changes accordingly.



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Recall the default panel setting

DEFAULT
SHIFT 2

Press the shift key, then 2 to recall the default panel setting.

The "done" message appears.



The panel is updated with the default setting.



Wave type	Sine wave
Frequency	10.0000kHz
TTL/CMOS	Disabled
–20dB	Disabled
Modulation	Disabled
Sweep mode	Disabled

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com


APPLICATION EXAMPLES

Reference Signal for PLL System

Description

The SFG output can be used as a cost-effective reference signal for Phase-Locked-Loop system. Directly connect SFG output to PLL input.

Block diagram

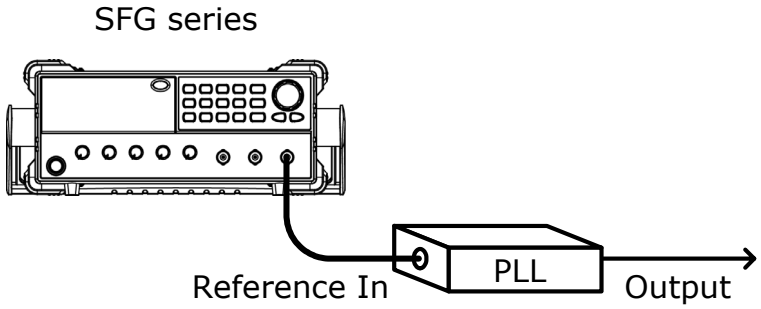


Trouble-Shooting Signal Source

Description

The SFG output can be used as the signal source to test the failed part in a circuit system. Isolate the problematic part from the rest, feed the SFG output as a stimulus, and observe the outcome using an oscilloscope.

Block diagram

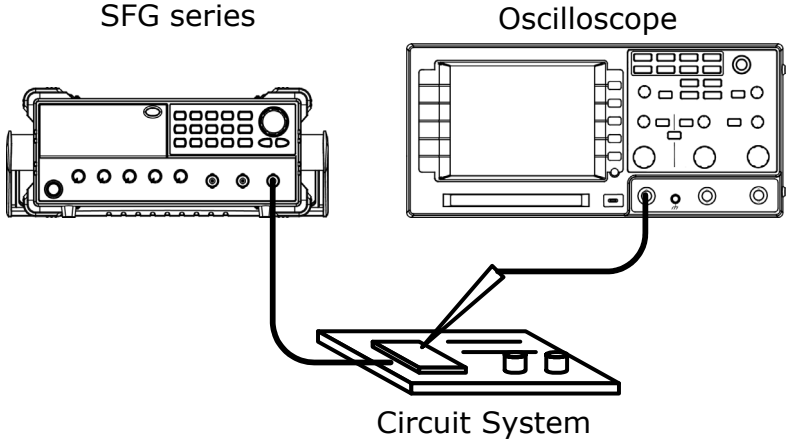


Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Transistor DC Bias Characteristics Test


Description

Use SFG-2000 series as the signal source for a transistor. Compare the transistor input/output waveform using the oscilloscope. Adjust the DC voltage source to find out the maximum output without distorting the waveform.

Block diagram

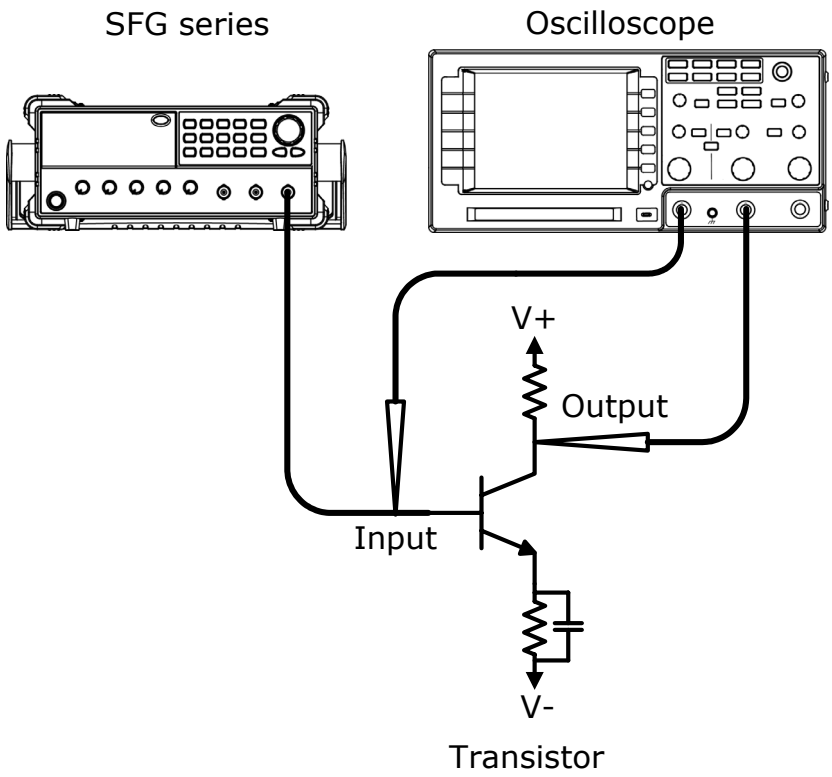

Oscilloscope display

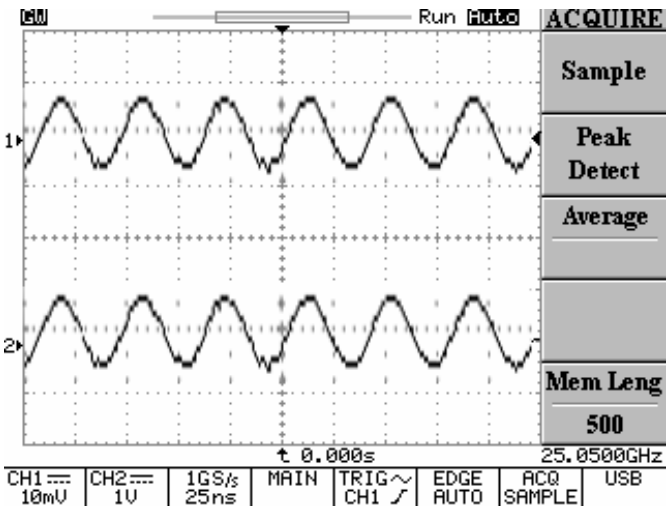


Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Amplifier Over-Load Characteristic Test

Description

Use the triangle wave output from SFG-2000 series to check the amplifier output distortion caused by overload. The common sine wave is not the ideal source in this case. Observe the linearity of the triangle waveform using an oscilloscope.

Block diagram

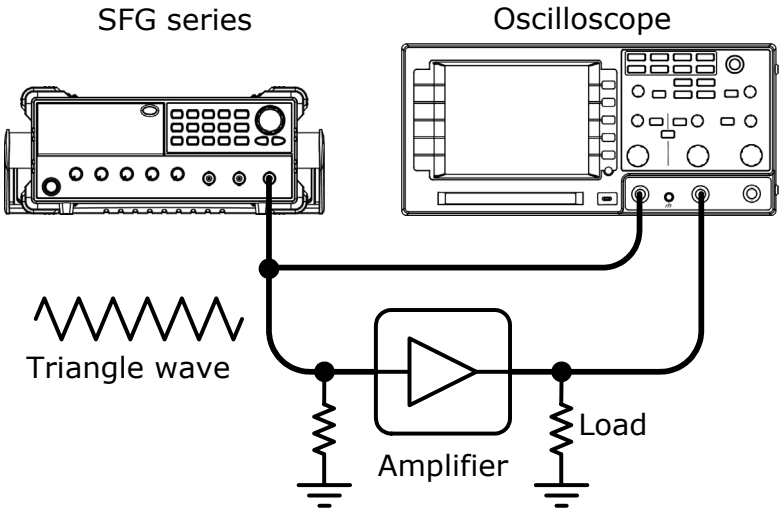


Amplifier Transient Characteristics Test

Description

Use the square wave output from SFG-2000 series to check the transient frequency response of an amplifier. The common sine wave is not the ideal source in this case. Observe the waveform using an oscilloscope.

Block diagram

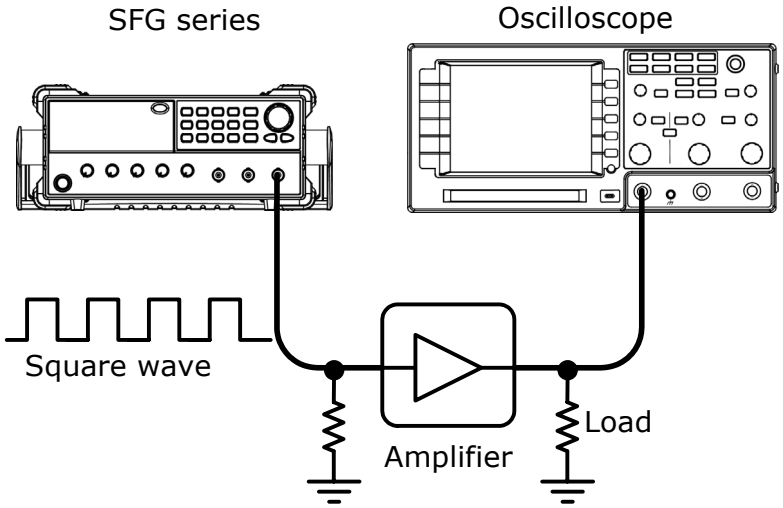

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Test step	1. Apply a triangle waveform to the amplifier first. Adjust the waveform amplitude to make sure there is no clipping. 2. Switch to square waveform and adjust its frequency to the middle of the amplifier pass band, such as 20Hz, 1kHz, and 10kHz. 3. Observe the shape of the amplifier output. The following table shows the possible output distortions and their explanations.

Transient characteristic list		• Amplitude reduction at low frequency • No phase shift
		• Low frequency boosted (accentuated fundamental)
		• High frequency loss • No phase shift
		• Low frequency phase shift • Trace thickened by hum-voltage
		• High frequency loss • Phase shift
		• Low frequency loss • Phase shift
		• Low frequency loss • Low frequency phase shift
		• High frequency loss • Low frequency phase shift
		• Damped oscillation

Note	For narrow band amplifier testing, square wave may not be suitable.


Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Logic Circuit Test

Description

Use the TTL/CMOS output from SFG-2000 series to test digital circuits. Observe the timing relation of input/output waveform using an oscilloscope.

Block diagram

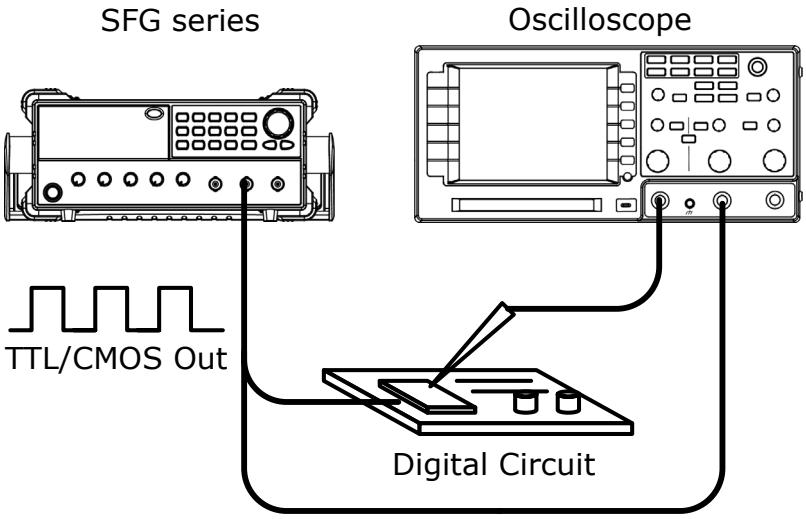


Impedance Matching Network Test

Description

Use SFG-2000 series for impedance matching network: testing its frequency characteristic and matching the impedance.

Block diagram

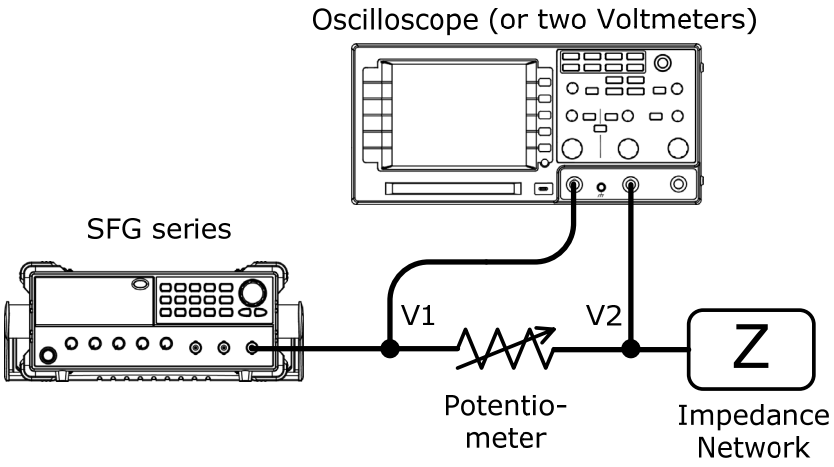

Test step

Adjust the potentiometer until V2 becomes the half of V1 (V2=0.5V1). Then the impedance Z of the network becomes identical to the potentiometer.


Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Speaker Driver Test

Description


Use SFG-2000 series for testing the frequency characteristics of audio speakers. Record the volt reading versus the input signal frequency.

Block diagram

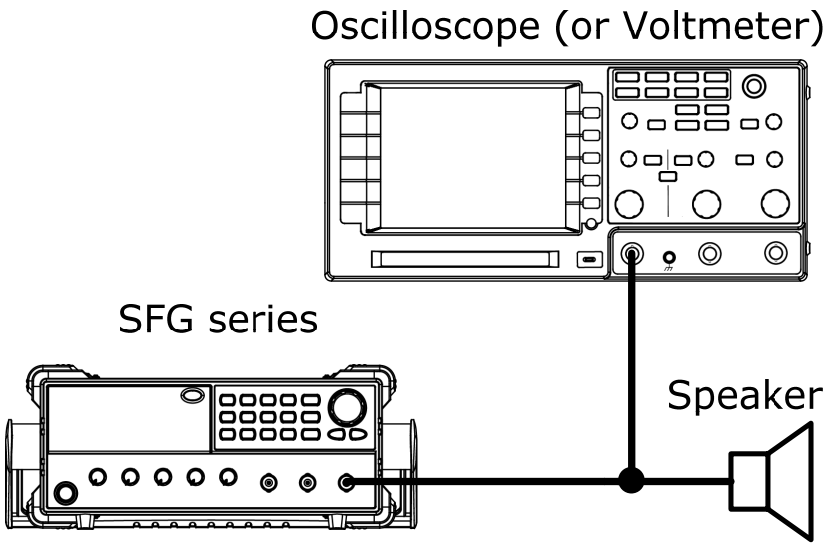


Graph

The peak voltage occurs on the resonant frequency of the speaker.

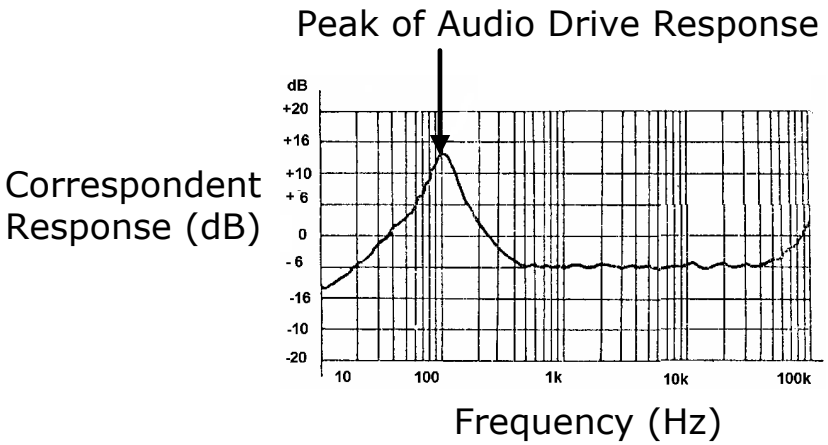

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Sweep for Speaker Test

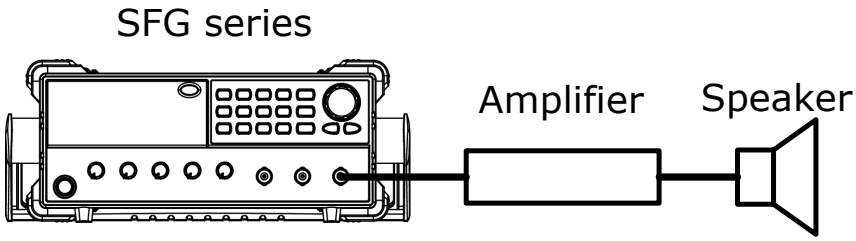Description	Use the sweep feature in SFG-2000 series for testing the frequency response of an audio speaker.
Test description	1. Set SFG output to sine wave, 20Hz. 2. Activate sweep and set LIN/LOG, sweep time, and sweep span. 3. Change the frequency if other bands need to be tested.
Block diagram	

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

FAQ

- I pressed the Power key on the front panel but nothing happens.
- How can I get out of Counter/Sweep/Modulation/TTL/−20dB mode?
- The device accuracy does not match the specification.
- What are these error messages?

I pressed the Power key on the front panel but nothing happens.

Make sure the AC source voltage setting on the rear panel is correct (page21). Otherwise the internal fuse might be blown out. Contact the service personnel.

How can I get out of Counter/Sweep/Modulation/TTL/−20dB mode?

Press the Shift key, then the relevant numerical key. (Do the same action as you entered those modes)

For example: To get out of Counter mode, press Shift then 1.

The device accuracy does not match the specification.

Make sure the device is powered On for at least 30 minutes, within +20°C~+30°C. This is necessary to stabilize the unit to match the specification.

What are these error messages?

Several messages appear when trying to set the frequency or duty cycle in forbidden way. Page52 summarizes all the error message content.

If there is still a problem, please contact your local dealer or GWInstek at www.gwinstek.com.tw / marketing@goodwill.com.tw.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

APPENDIX

Error Messages

Frequency error

FrEq-Err

FrEq-Err1	Sine and square wave frequency over range. This message appears when entering sine or square waveform frequency larger than the rating. See page26 for sine/square rating.
FrEq-Err2	Triangle wave Frequency over range. This message appears when entering triangle waveform frequency larger than 1MHz. See page26 for triangle wave rating.
FrEq-Err3	FM Center Frequency over range. This message appears when trying to enter FM center frequency larger than specified. See page38 for FM center frequency range.

Duty Cycle error

duty-Err

duty-Err1	Not square waveform. This message appears when trying to set duty cycle in non-square (=sine or triangle) waveform. For duty cycle setting, see page28 (square wave) or page33 (TTL/CMOS output).
duty-Err2	Square wave frequency over range. This message appears when trying to set duty cycle when the square wave frequency is over 1MHz. For square wave frequency setting, see page26.
duty-Err3	Duty over range. This message appears when the duty cycle setting goes outside 20~80% range. For duty cycle range, see page28 (square wave) or page33 (TTL/CMOS output).

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Specification

Main	Output Function	Sine, Square, Triangle	
	Amplitude Range	10Vp-p (into 50Ω load)	
	Impedance	50Ω ± 10%	
	Attenuator	−20dB ± 1dB x2	
	DC Offset	< −5V ~ >+5V (50Ω load)	
	Duty Range	20% ~ 80%, 2Hz~1MHz (Square Wave)	
	Duty Resolution	1% (Square Wave Only)	
	Display	9 digits LED display	
Frequency	Sine/Square Waveform Range	SFG-2004	0.1Hz ~ 4MHz
		SFG-2007	0.1Hz ~ 7MHz
		SFG-2010	0.1Hz ~ 10MHz
		SFG-2020	1Hz ~ 20MHz
		SFG-2104	0.1Hz ~ 4MHz
		SFG-2107	0.1Hz ~ 7MHz
		SFG-2110	0.1Hz ~ 10MHz
		SFG-2120	1Hz ~ 20MHz
	Triangle Waveform Range	0.1Hz ~ 1MHz (1Hz ~ 1MHz for SFG-2020/2120)	
	Resolution	0.1Hz (1Hz for SFG-2020/2120)	
	Stability	±20ppm	
	Accuracy	±20ppm	
	Aging	±5ppm/year	
Sine Wave	Harmonic Distortion	≥−55dBc, 0.1Hz ~ 200kHz ≥−40dBc, 0.2MHz ~ 4MHz ≥−30dBc, 4MHz ~ 20MHz (Amplitude at maximum position without attenuating 1/10 of any combination setting, TTL/CMOS off)	
	Flatness	< ± 0.3dB, 0.1Hz ~ 1MHz < ± 0.5dB, 1MHz ~ 4MHz < ± 2dB, 4MHz ~ 10MHz < ± 3dB, 10MHz ~ 20MHz (At the max amplitude relating to 1kHz)	
Triangle Wave	Linearity	≥ 98%, 0.1Hz ~ 100kHz ≥ 95%, 100kHz ~ 1MHz	
Square Wave	Symmetry	±1% of period + 4ns, 0.1Hz ~ 100kHz	
	Rise/Fall Time	≤ 25ns at maximum output (50Ω load)	
CMOS Output	Level	4 ± 1Vpp ~ 15 ± 1Vpp, adjustable	
	Rise/Fall Time	≤ 120ns	

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

TTL Output	Level	≥ 3Vpp
	Fan Out	20 TTL Load
	Rise/Fall Time	≤ 25ns
Sweep (SFG-2100 Series)	Sweep Rate	100:1 Ratio Max, adjustable (Note1)
	Sweep Time	1 ~ 30s, adjustable (Note2)
	Sweep Mode	Linear, Logarithmic
Amplitude Modulation (SFG-2100 Series)	Depth	0 ~ 100%
	Frequency	400Hz (internal), DC ~ 1MHz (external)
	Carrier BW	100Hz ~ 5MHz (−3dB)
	External Modulating	Sensitivity: ≤ 10Vpp for 100% modulation
Frequency Modulation (SFG-2100 Series)	Deviation	≥0 ~ ±50kHz, center at 1MHz
	Frequency	400Hz fixed (internal), 1kHz fixed (external)
	External Modulating	Sensitivity: ≤ 10Vpp for 10% modulation (center at 1MHz)
Frequency Counter (SFG-2100 Series)	Range	5Hz ~ 150MHz
	Accuracy	Time Base Accuracy ± 1 count
	Time Base	±20ppm (23±5°C) after 30min warmup
	Max. Resolution	100nHz for 1Hz, 0.1Hz for 100MHz
	Input Impedance	1MΩ/150pf
	Sensitivity	≤ 35mVrms, 5Hz ~ 100MHz ≤ 45mVrms, 100MHz ~ 150MHz
Store/Recall	10 Groups of Setting Memories	
General	Power Source	AC115V/230V +10%, −15%, 50/60Hz
	Operation Environment	Indoor Use, Altitude Up to 2000m Ambient Temperature 0 ~ 40°C Relative Humidity ≤ 80%, 0 ~ 40°C Relative Humidity ≤ 70%, 35 ~ 40°C Install Category II / Pollution Degree 2
	Storage Environment	Temperature: −10 ~ 70°C Humidity: ≤70%
	Accessories	Instruction Manual x 1, Power Cord x 1 GTL-101 x 2 (SFG-2100 Series) GTL-101 x 1 (SFG-2000 Series)
	Dimension	107 (W) x 266 (H) x 293 (D)
	Weight	Approx. 3.2kg (SFG-2100 Series) Approx. 3.1kg (SFG-2000 Series)

Note1: In order to get the maximum sweep span, sweep time needs to be tuned.
Note2: If sweep time is too long, the stop frequency will stay at the maximum frequency until the end of the sweep cycle.

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Declaration of Conformity

We
GOOD WILL INSTRUMENT CO., LTD.
(1) No.7-1, Jhongsing Rd., Tucheng City, Taipei County, Taiwan
(2) No. 69, Lu San Road, Suzhou City (Xin Qu), Jiangsu Sheng, China
declare, that the below mentioned product
Type of Product: Synthesized Function Generator
Model Number: SFG-2004, SFG-2007, SFG-2010, SFG-2020, SFG-2104, SFG-2107, SFG-2110, SFG-2120
are herewith confirmed to comply with the requirements set out in the Council Directive on the Approximation of the Law of Member States relating to Electromagnetic Compatibility (89/336/EEC, 92/31/EEC, 93/68/EEC) and Low Voltage Directive (73/23/EEC, 93/68/EEC).
For the evaluation regarding the Electromagnetic Compatibility and Low Voltage Directive, the following standards were applied:

◎ **EMC**

EN 61326-1: Electrical equipment for measurement, control and laboratory use — EMC requirements (1997 + A1:1998 + A2:2001 + A3:2003)	
Conducted Emission Radiated Emission EN 55011: Class A 1998 + A1:1999 + A2:2002	Electrostatic Discharge EN 61000-4-2: 1995 + A1:1998 + A2:2001
Current Harmonics EN 61000-3-2: 2000 + A2:2005	Radiated Immunity EN 61000-4-3: 2002 + A1:2002
Voltage Fluctuations EN 61000-3-3: 1995 + A1:2001	Electrical Fast Transients EN 61000-4-4: 2004
----------	Surge Immunity EN 61000-4-5: 1995 + A1:2001
----------	Conducted Susceptibility EN 61000-4-6: 1996 + A1:2001
----------	Power Frequency Magnetic Field EN 61000-4-8: 1993 + A1:2001
----------	Voltage Dip/ Interruption EN 61000-4-11: 2004

◎ **Safety**

Low Voltage Equipment Directive 73/23/EEC & amended by 93/68/EEC
Safety Requirements IEC/EN 61010-1: 2001

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

INDEX

2

20dB attenuation 29
example setting 22

A

AM
example setting 23
setup 37
amplifier application example 46
application examples 44

C

cleaning 7
CMOS
activation 32
example setting 22
constant current circuit 10
control knob overview 17
counter gate time 40
counter input 40
example setting 24

D

DDS block diagram 11
default panel setting
contents 43
recall 43
default setting
contents 24
default setting recall 21
direct digital synthesis 10
display contents overview 14
duty cycle
example setting 22
setup 28
duty cycle error 28, 52
faq 51

E

EN 61010 ..... 6, 7, 55
EN55011 55
EN61000 55
external modulation 37, 39
example setting 23

F

FAQ 51
FM
example setting 23
seup 38
frequency
editing 27
entering 26
frequency error 27, 39, 52
faq 51
front panel diagram
SFG-2000 13
SFG-2100 13
fuse
safety instruction 6

I

impedance application example 48
in/out terminal overview 16

L

lin sweep selection 35
log sweep selection 35
logic application example 48

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

M

main feature list 12
memory recall
  example setting 24
memory store
  example setting 24
model lineup 12

N

numerical keys overview 15

O

offset 30
  example setting 22
operation environment
  safety instruction 7
operation shortcuts 22

P

phase locked loop
  example application 44
power supply
  safety instruction 6
power up sequence 21
  FAQ 51

R

rear panel 19
recall setting 42

S

safety
  guidelines 6
  symbol 5
  UK power cord 8
setup step 20
sine wave
  example setting 22
  selection 26
speaker application example 49, 50
specification 53
  FAQ 51
square wave
  duty cycle 28
  example setting 22
  selection 26
storage environment
  safety instruction 7
store setting 42
sweep
  example setting 23
  setup 35

T

table of contents 3
technical background 10
tilt stand 20
transistor application example 45
triangle wave
  example setting 22
  selection 26
troubleshooting application example 44
TTL
  activation 32
  example setting 22

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Artisan Technology Group is an independent supplier of quality pre-owned equipment

Gold-standard solutions

Extend the life of your critical industrial, commercial, and military systems with our superior service and support.

We buy equipment

Planning to upgrade your current equipment? Have surplus equipment taking up shelf space? We'll give it a new home.

Learn more!

Visit us at **artisantg.com** for more info on price quotes, drivers, technical specifications, manuals, and documentation.

Artisan Scientific Corporation dba Artisan Technology Group is not an affiliate, representative, or authorized distributor for any manufacturer listed herein.

We're here to make your life easier. How can we help you today?

(217) 352-9330 | sales@artisantg.com | artisantg.com

ARTISAN® TECHNOLOGY GROUP