

ARTISAN®
TECHNOLOGY GROUP

Your **definitive** source for quality pre-owned equipment.

**Artisan Technology Group**
(217) 352-9330 | sales@artisantg.com | artisantg.com

**Full-service, independent repair center**
with experienced engineers and technicians on staff.

**We buy your excess, underutilized, and idle equipment**
along with credit for buybacks and trade-ins.

**Custom engineering**
so your equipment works exactly as you specify.

- Critical and expedited services
- In stock / Ready-to-ship
- Leasing / Rentals / Demos
- ITAR-certified secure asset solutions

**Expert team | Trust guarantee | 100% satisfaction**

All trademarks, brand names, and brands appearing herein are the property of their respective owners.

Find the *National Instruments PXIe-4302* at our website: ***Click HERE***

DEVICE SPECIFICATIONS

# NI PXIe-4302/4303

32 Ch, 24-bit, 5 kS/s or 51.2 kS/s Simultaneous Filtered Data Acquisition Module

Français Deutsch 日本語 한국어 简体中文

ni.com/manuals

This document lists specifications for the NI PXIe-4302/4303 simultaneous filtered data acquisition module. All specifications are subject to change without notice. Visit `ni.com/manuals` for the most current specifications and product documentation.

**Note** To maintain forced air cooling in the PXIe system, refer to the *Maintain Forced-Air Cooling Note to Users*.

## Terminology

*Maximum* and *minimum* specifications characterize the warranted performance of the instrument within the recommended calibration interval and under the stated operating conditions. These specifications are subject to production verification or guaranteed by design.

*Typical* specifications are specifications met by the majority of the instruments within the recommended calibration interval and under the stated operating conditions, based on measurements taken during production verification and/or engineering development. The performance of the instrument is not warranted.

*Supplemental* specifications describe the basic function and attributes of the instrument established by design and are not subject to production verification. They provide information that is relevant for the adequate use of the instrument that is not included in the previous definitions.

All performance specifications are *typical* unless otherwise noted. These specifications are valid within the full operating temperature range. Accuracy specifications are valid within ±5 °C of the calibration or over the full operating range as specifically noted.

## Input Characteristics

Number of channels..... 32 differential analog input channels

ADC resolution..... 24 bits

Type of ADC..... Delta-Sigma

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Sampling mode ..... Simultaneous

Sample rates ($f_s$)

NI PXIe-4302

Range ..... 1 S/s to 5 kS/s

Resolution ..... ≤181.9 µS/s

NI PXIe-4303

Range ..... 1 S/s to 51.2 kS/s

Resolution ..... ≤181.9 µS/s

Input coupling ..... DC

Input ranges (FS)

10 V range

Nominal ..... ±10 V

Typical ..... ±10.34 V

Minimum ..... ±10.26 V

100 mV range

Nominal ..... ±100 mV

Typical ..... ±103.4 mV

Minimum ..... ±102.4 mV

Maximum working voltage (signal + common mode)

10 V range ..... ±10.4 V

100 mV range ..... ±8.5 V

Input impedance

Device powered on

AI+ to AI GND ..... >1 GΩ

AI- to AI GND ..... >1 GΩ

Input bias current ..... ±1.5 nA

CMRR (DC to 60 Hz)

10 V range ..... 85 dB

100 mV range ..... 125 dB

FIFO Buffer Size ..... 1,023 samples

Data transfers ..... Direct memory access (DMA), programmed I/O

## Fault Protection (Power On or Off)

AI±<0..31>, AIGND ..... 30 V between any two pins

PFI0 ..... 30 V to DGND



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

## Accuracy[1]

| Measurement Conditions | Range: 10 V | |
|---|---|---|
| | Gain Error (% of Reading) | Offset Error (μV) |
| Typ (23 °C ±5 °C) | 0.025 | 859 |
| Max (23 °C ±5 °C) | 0.031 | 1262 |
| Max (0 °C to 55 °C) | 0.062 | 2897 |

| Measurement Conditions | Range: 100 mV | |
|---|---|---|
| | Gain Error (% of Reading) | Offset Error (μV) |
| Typ (23 °C ±5 °C) | 0.032 | 17 |
| Max (23 °C ±5 °C) | 0.043 | 29 |
| Max (0 °C to 55 °C) | 0.087 | 68 |

## Temperature Stability

Range: 10 V

Gain stability..... 8 ppm/°C

Offset stability ..... 31 μV/°C

Range: 100 mV

Gain stability..... 10 ppm/°C

Offset stability ..... 0.76 μV/°C

[1] Accuracies listed are warranted for the conditions described in the tables and for up to one year from the module external calibration.



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

# Input Noise

**Table 1.** Total Buffered Mode Noise

| Measurement Range | $f_s$ = 5 kS/s | $f_s$ = 51.2 kS/s* |
|---|---|---|
| 10 V Range | 22 $\mu V_{rms}$ | 70 $\mu V_{rms}$ |
| 100 mV Range | 1 $\mu V_{rms}$ | 3.2 $\mu V_{rms}$ |
| *NI PXIe-4303 only. | | |

**Table 2.** Optional Buffered Mode IIR Filtering Noise Scaling Coefficients

| Filter Cut-Off Frequency | Noise Scaling Coefficient (K) |
|---|---|
| 2 kHz | 1.1 |
| 1 kHz | 1.8 |
| 200 Hz | 3 |
| 20 Hz | 12 |
| 2 Hz | 30 |

Buffered mode noise with IIR filters

$$Input\ Noise = \frac{Total_Buffer_Mode_Noise}{\sqrt{Highest_Rate \times \frac{Hz}{S/s} \times 0.45}} \times \sqrt{K \times Filter_Cut\text{-}off_Frequency}$$

Example

When using the 10 V range, the buffer mode noise of the NI PXIe-4303 with the 1 kHz optional IIR filter is:

Highest_Rate of the NI PXIe-4303 = 51.2 kS/s

Total_Buffer_Mode_Noise = 70 $\mu V_{rms}$

Noise Scaling Coefficient (K) of 1 kHz filter = 1.8

K × Filter_Cut-off_Frequency= 1.8 × 1 kHz = 1.8 kHz

$$Input\ Noise = \frac{Total_Buffer_Mode_Noise}{\sqrt{Highest_Rate \times \frac{Hz}{S/s} \times 0.45}} \times \sqrt{K \times Filter_Cut\text{-}off_Frequency}$$

$$= \frac{70\ \mu V_{rms}}{\sqrt{51.2\ kS/s \times \frac{Hz}{S/s} \times 0.45}} \times \sqrt{1.8\ kHz} = 19.6\ \mu V_{rms}$$



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

# Absolute Accuracy

$$Absolute\ Accuracy = Reading \times Gain\ Error + Offset\ Error + Noise\ Uncertainty$$

$$Noise\ Uncertainty = 3 \times \frac{Random\ Noise}{\sqrt{\#\ Samples}}$$

where

*Random Noise* is the input noise for the sample rate used.

3 converts the RMS value to peak value for a coverage of 3σ.

*# Samples* is the number of samples averaged

For example, when using an operating temperature of 23 °C ±5 °C with the 10 V range, the absolute accuracy at full-scale input with 5000 samples acquired at 5 kS/s is:

$$Gain\ Error = 0.031\%\ of\ Reading$$

$$Offset\ Error = 1262\ \mu V$$

$$Noise\ Uncertainty = \frac{22\ \mu V \times 3}{\sqrt{5000}} = 0.9\ \mu V$$

$$Absolute\ Accuracy = 10\ V \times Gain\ Error + Offset\ Error + Noise\ Uncertainty = 4362\ \mu V$$

Phase linearity

NI PXIe-4302
($f_{in}$ = DC to 2.25 kHz)..... ±1°

NI PXIe-4303
($f_{in}$ = DC to 23.04 kHz)..... ±1°

Spurious free dynamic range (SFDR)

1 kHz, -60 dBFS ..... 120 dB

Total harmonic distortion (THD)

10 V range
1 kHz, -1 dBFS ..... -98 dB

100 mV range
1 kHz, -1 dBFS ..... -98 dB

Crosstalk

1 kHz..... -95 dB

10 kHz..... -75 dB (NI PXIe-4303 only)



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

# Bandwidth and Alias Rejection

Passband

Frequency (for 1 S/s ≤ $f_s$ < 25 S/s) ..... ≤0.1 × $f_s$

Frequency (for 25 S/s ≤ $f_s$ ≤ 25.6 kS/s) .... ≤0.45 × $f_s$

**Table 3.** In Band Flatness

| Measurement Range | $f_{in}$ = DC to 2.25 kHz | $f_{in}$ = 2.25 kHz to 23.04 kHz* |
|---|---|---|
| 10 V Range | 10 mdB max | 100 mdB max |
| 100 mV Range | 30 mdB max | 300 mdB max |
| *NI PXIe-4303 only. | | |

Stopband

Frequency (for 1 S/s ≤ $f_s$ < 25 S/s) ..... ≤0.9 × $f_s$

Frequency (for 25 S/s ≤ $f_s$ ≤ 25.6 kS/s) .... ≤0.57 × $f_s$

Rejection ..... 100 dB

Alias-free bandwidth
(for 1 S/s ≤ $f_s$ < 25 S/s) ..... 0.1 × $f_s$

Alias-free bandwidth
(for 25 S/s ≤ $f_s$ ≤ 25.6 kS/s) ..... 0.45 × $f_s$

Minimum frequency
for ADC alias hole ..... 3.320313 MHz

Rejection at alias hole ..... 100 dB

Uncompensated filter delay[1]

*Group Delay = Analog Delay + Digital Filter Group Delay* [2]

Analog delay

10 V range ..... 6.77 µs

100 mV range ..... 7.76 µs

[1] The compensated digital filter group delay is a result of using the anti-alias filtering in buffered mode. Hardware automatically compensates for this group delay when synchronizing. Hardware does not compensate for filter delay from either the analog filter or the optional buffered mode digital filter or the filter used for hardware-timed single point mode.

[2] Digital filter group delay results from using the optional IIR filter in buffered mode or the IIR filter selected in hardware-timed single point mode.



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Compensated digital filter group delay ..... 1.79742 ms + Variable Filter Delay

| Sample Rate | Variable Filter Delay (Samples) |
|---|---|
| 1 S/s ≤ $f_s$ < 25 S/s | 4.000 |
| 25.0 S/s ≤ $f_s$ ≤ 25.3 S/s | 57.995 |
| 25.3 S/s < $f_s$ ≤ 50.7 S/s | 57.991 |
| 50.7 S/s < $f_s$ ≤ 101.3 S/s | 57.981 |
| 101.3 S/s <$f_s$ ≤ 202.7 S/s | 57.963 |
| 202.7 S/s < $f_s$ ≤ 405.3 S/s | 57.926 |
| 405.3 S/s < $f_s$ ≤ 810.6 S/s | 57.852 |
| 810.6 S/s < $f_s$ ≤ 1621.2 S/s | 57.703 |
| 1621.2 S/s < $f_s$ ≤ 3242.5 S/s | 57.406 |
| 3242.5 S/s < $f_s$ ≤ 6485.0 S/s | 56.813 |
| 6485.0 S/s < $f_s$ ≤ 12970.0 S/s | 55.625 |
| 12970.0 S/s < $f_s$ ≤ 25939.9 S/s | 53.250 |
| 25939.9 S/s < $f_s$ ≤ 51200 S/s | 48.500 |

# Channel to Channel Matching[1]

**Table 4.** Gain Matching

| Measurement Range | Input Signal Frequency ($f_{in}$) | |
|---|---|---|
| | DC to 2.25 kHz | 2.25 kHz to 23.04 kHz* |
| 10 V Range | 17 mdB max | 170 mdB max |
| 100 mV Range | 34 mdB max | 340 mdB max |
| * NI PXIe-4303 only. | | |

Phase matching

10 V range ..... $\frac{0.035°}{\text{kHz}} \times f_{in}$

100 mV range ..... $\frac{0.045°}{\text{kHz}} \times f_{in}$

[1] Identical channel configurations.




Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

# Optional Buffered Mode IIR Filtering

| Filter Cut-Off Frequency | Filter Type | Stopband Attenuation | Passband Ripple |
|---|---|---|---|
| 2 kHz Filter | Fourth order, Elliptic Filter | -120 dB | 0.2 dB |
| 1 kHz Filter | Fourth order, Elliptic Filter | -120 dB | 0.2 dB |
| 200 Hz Filter | Fourth order, Elliptic Filter | -120 dB | 0.2 dB |
| 20 Hz Filter | Fourth order, Elliptic Filter | -120 dB | 0.2 dB |
| 2 Hz Filter | Fourth order, Elliptic Filter | -120 dB | 0.2 dB |

**Figure 1.** Magnitude Response

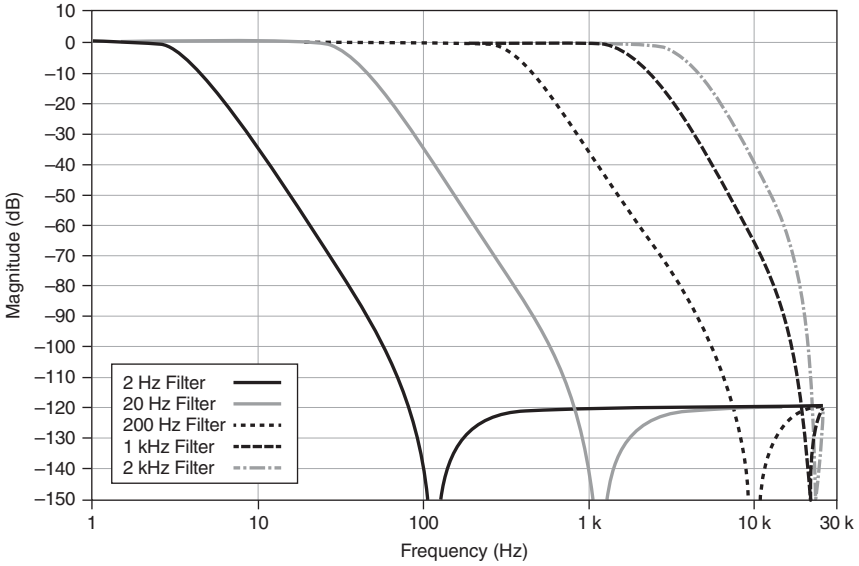




Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

**Figure 2.** Passband


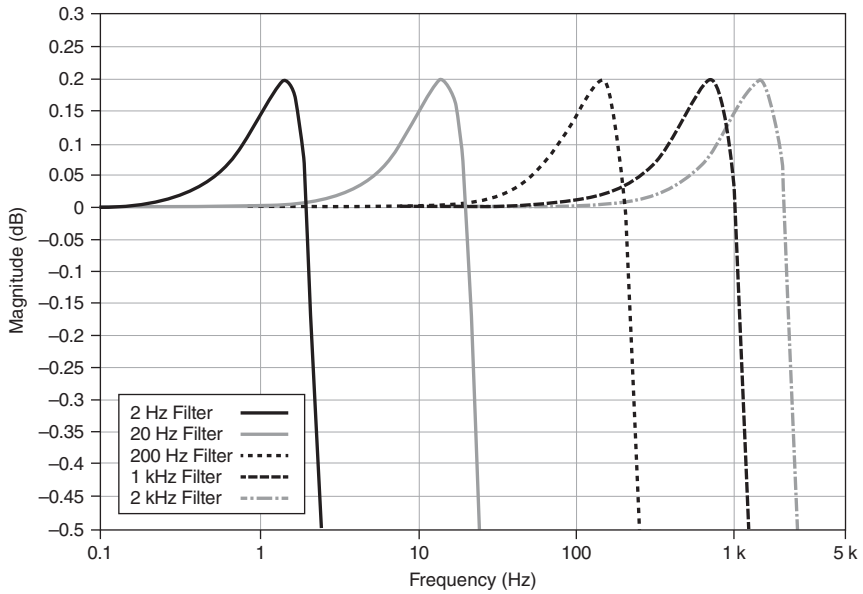



**Figure 3.** Phase Response



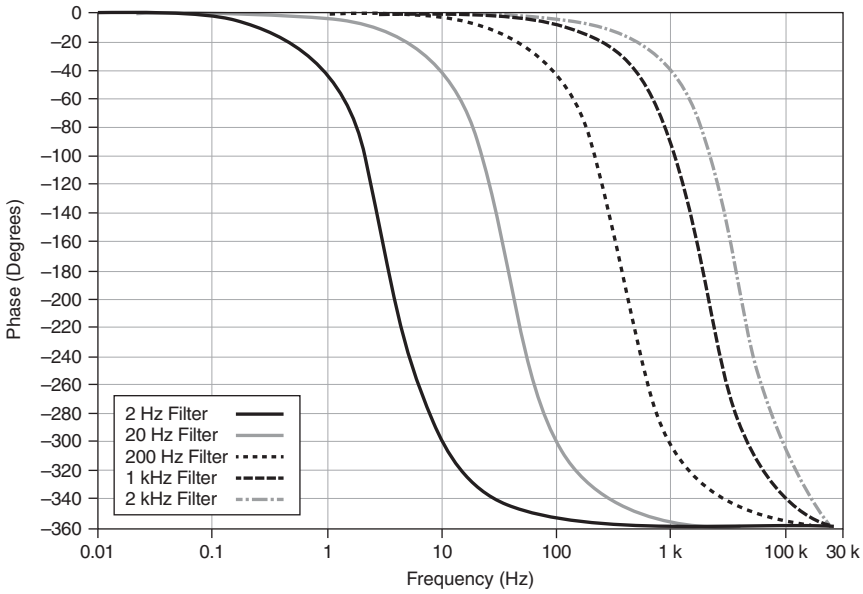


Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

**Figure 4.** Group Delay

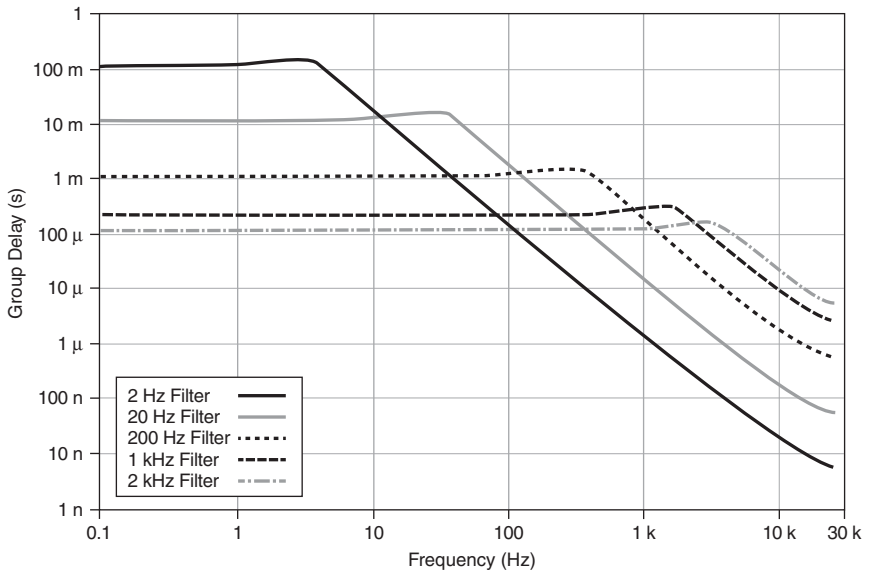



**Table 5.** Digital Filter Group Delay

| Filter Cut-Off Frequency | Group Delay at 0.1 Hz |
|---|---|
| 2 kHz Filter | 113.4 µs |
| 1 kHz Filter | 227.4 µs |
| 200 Hz Filter | 1.1385 ms |
| 20 Hz Filter | 11.3856 ms |
| 2 Hz Filter | 113.856 ms |



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

# Hardware-Timed Single Point Sample Mode

Acquisition rate[1]

Minimum ..... 1 S/s

Maximum

NI PXIe-4302 ..... 5 kS/s

NI PXIe-4303 ..... 51.2 kS/s

**Table 6.** Measured Hardware-Timed Single Point Sample Mode Noise at 23 °C

| Filter Cut-Off Frequency | 10 V Range | 100 mV Range |
|---|---|---|
| 3 kHz Filter | 31.8 $\mu V_{rms}$ | 1.0 $\mu V_{rms}$ |
| 2 kHz Filter | 29.7 $\mu V_{rms}$ | 906 $nV_{rms}$ |
| 1 kHz Filter | 27.2 $\mu V_{rms}$ | 661 $nV_{rms}$ |
| 500 Hz Filter | 25.6 $\mu V_{rms}$ | 492 $nV_{rms}$ |
| 200 Hz Filter | 24.7 $\mu V_{rms}$ | 357 $nV_{rms}$ |
| 100 Hz Filter | 24.6 $\mu V_{rms}$ | 300 $nV_{rms}$ |

# Hardware-Timed Single Point Filtering

Filter type..... Fourth order, elliptic filter

Stopband attenuation ..... -120 dB

Passband ripple..... 0.2 dB

[1] Depends on the system setup and application time. Refer to the *NI PXIe-4302/4303 User Manual* for more information.



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

**Figure 5.** Filter Magnitude Response


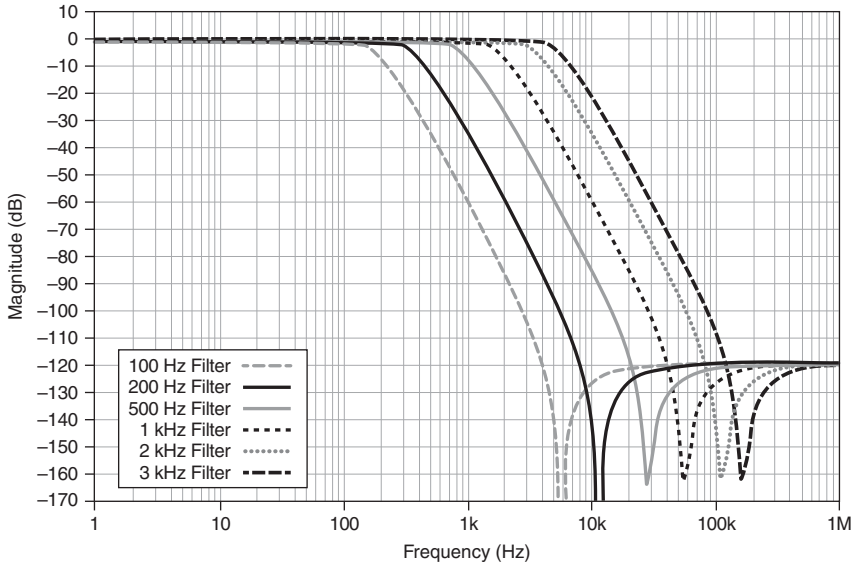



**Figure 6.** Passband Ripple



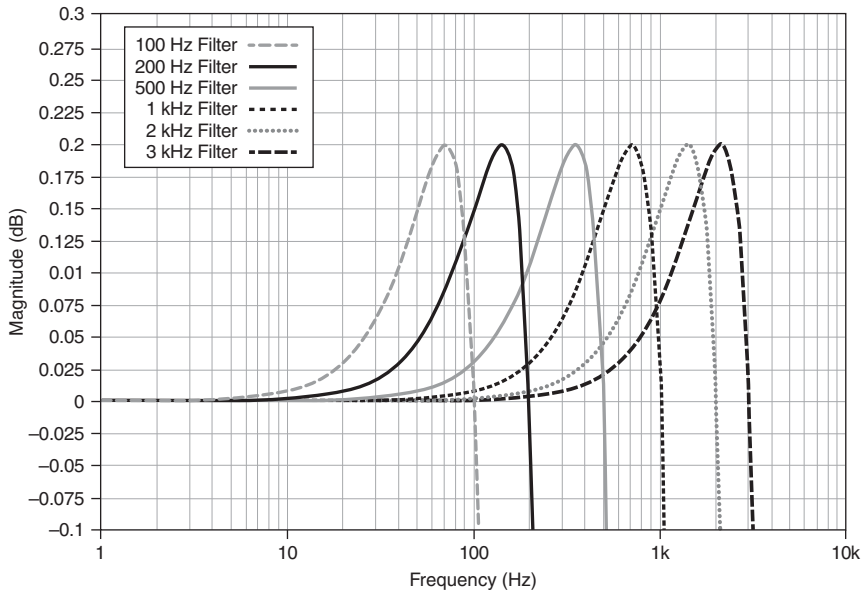


Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

**Figure 7.** Filter Phase Response


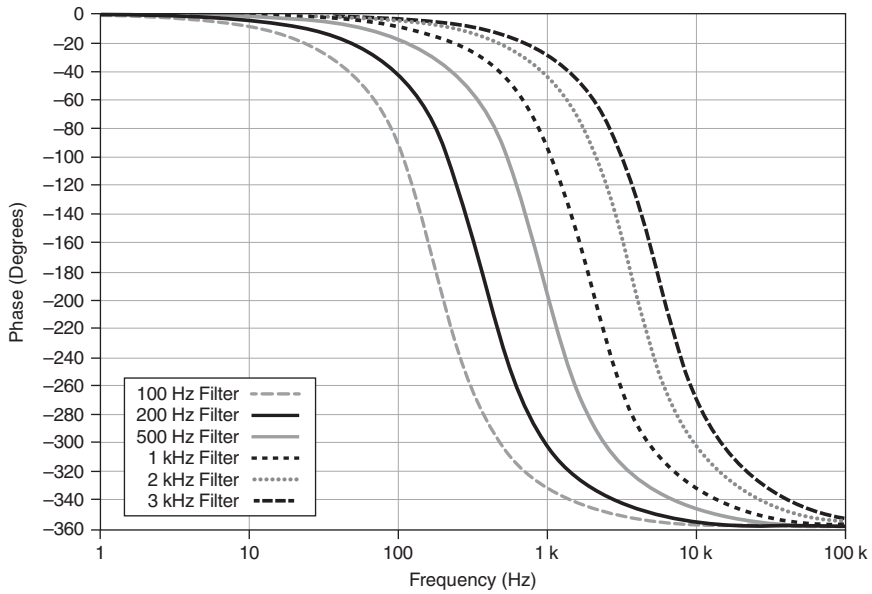



**Figure 8.** Filter Group Delay



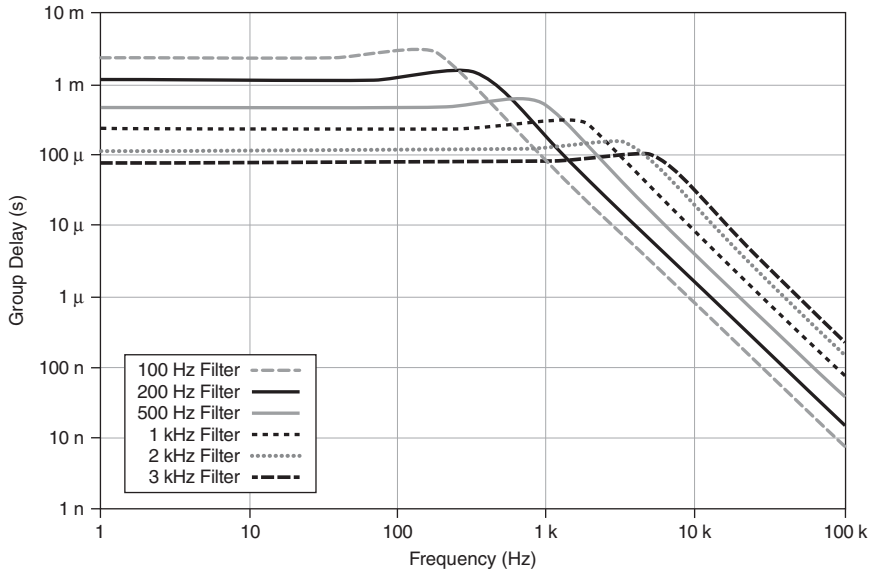


Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

**Table 7.** Digital Filter Group Delay

| Filter Cut-Off Frequency | Group Delay at 1 Hz |
|---|---|
| 3 kHz Filter | 75.9 µs |
| 2 kHz Filter | 113.9 µs |
| 1 kHz Filter | 227.7 µs |
| 500 Hz Filter | 455.4 µs |
| 200 Hz Filter | 1.1386 ms |
| 100 Hz Filter | 2.28 ms |

Hardware-timed single point ADC group delay[1] ..... 1.6 µs

## Internal Frequency Timebase Characteristics

Frequency ..... 106.25 MHz

Accuracy ..... ±50 ppm

## Synchronization

Reference clock source ..... Onboard 106.25 MHz clock, Backplane PXIe_CLK100

## Task Resources[2]

Timing engines ..... 4

Buffered mode streams ..... 4

Hardware-timed single point streams ..... 4

Maximum channels per stream ..... 8

[1] When in hardware-timed single point mode, *Total group delay = ADC group delay + Filter group delay.*

[2] The NI PXIe-4302/4303 can operate four independent timing engines simultaneously. Each timing engine can utilize one or more buffered mode or hardware-timed single point streams, but not both types simultaneously. Refer to the *NI PXIe-4302/4303 User Manual* for more details about timing engines and DSP streams.



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

# Triggers

Analog trigger

- Purpose ..... Reference trigger only
- Source ..... AI<0..31>
- Level ..... Full scale (depending on input range), programmable
- Mode ..... Rising-edge, Rising-edge with hysteresis, Falling-edge, Falling-edge with hysteresis, Entering Window, Leaving Window
- Resolution ..... 24 bits

Digital trigger

- Purpose ..... Start or reference trigger
- Source ..... PFI0, PXI_TRIG <0..7>, PXI_STAR, PXIe_DSTAR <A..B>
- Polarity ..... Software-selectable
- Minimum pulse width ..... 100 ns for PXI_TRIG <0..7>, 20 ns for others

# Output Timing Signals

Sources ..... Sample Clock, Start Trigger Out, Reference Trigger Out

Destinations ..... PFI0, PXI_TRIG <0..7>, PXIe_DSTARC

Polarity ..... Software-selectable

# PFI Characteristics

Input

- Logic compatibility ..... 3.3 V to 5 V
- High, $V_{IH}$ ..... 2.40 V
- Low, $V_{IL}$ ..... 0.95 V
- Input impedance ..... 10 kΩ

Output

- High, $V_{OH}$ ..... 3.43 V max
- Sourcing 5 mA ..... 2.88 V min
- Low, $V_{OL}$ sinking 5 mA ..... 0.33 V max
- Output impedance ..... 50 Ω
- Output current ..... ±5 mA min



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

## Bus Interface

Form factor ..... x1 PXI Express peripheral module, Specification rev 1.0 compliant

Slot compatibility ..... PXI Express or PXI Express hybrid slots

DMA channels ..... 4, analog input

## Calibration

You can obtain the calibration certificate and information about calibration services for the NI PXIe-4302/4303 at `ni.com/calibration`.

Recommended warm-up time ..... 15 minutes

Calibration interval ..... 1 year

## Power Requirement

+12 V ..... 1.3 A

+3.3 V ..... 1.1 A

## Physical Requirements

Dimensions ..... Standard 3U PXIe, 16 cm × 10 cm (6.3 in. × 3.9 in.)

Weight ..... 156 g (5.5 oz)

I/O connector ..... 96-pin male DIN 41612/IEC 60603-2 connector

**Caution** Clean the hardware with a soft, nonmetallic brush. Make sure that the hardware is completely dry and free from contaminants before returning it to service.

## Environmental Specifications

Maximum altitude ..... 2,000 m (800 mbar)

Pollution Degree ..... 2

Indoor use only.



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

## Operating Environment

Ambient temperature range ..... 0 °C to 55 °C
(Tested in accordance with IEC 60068-2-1 and IEC 60068-2-2. Meets MIL-PRF-28800F Class 3 low temperature limit and MIL-PRF-28800F Class 2 high temperature limit.)

Relative humidity range..... 10% to 90%, noncondensing
(Tested in accordance with IEC 60068-2-56.)

## Storage Environment

Ambient temperature range ..... -40 °C to 71 °C
(Tested in accordance with IEC 60068-2-1 and IEC 60068-2-2. Meets MIL-PRF-28800F Class 3 limits.)

Relative humidity range..... 5% to 95%, noncondensing
(Tested in accordance with IEC 60068-2-56.)

# Shock and Vibration

Operating shock ..... 30 g peak, half-sine, 11 ms pulse
(Tested in accordance with IEC 60068-2-27. Meets MIL-PRF-28800F Class 2 limits.)

Random vibration

- Operating ..... 5 Hz to 500 Hz, 0.3 $g_{rms}$
- Non-operating ..... 5 Hz to 500 Hz, 2.4 $g_{rms}$

(Tested in accordance with IEC 60068-2-64. Non-operating test profile exceeds the requirements of MIL-PRF-28800F, Class 3.)

# Safety

This product meets the requirements of the following standards of safety for electrical equipment for measurement, control, and laboratory use:

- IEC 61010-1, EN 61010-1
- UL 61010-1, CSA 61010-1

**Note** For UL and other safety certifications, refer to the product label or the *Online Product Certification* section.

**Caution** The protection provided by the NI PXIe-4302/4303 can be impaired if it is used in a manner not described in this documents.



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

# Electromagnetic Compatibility

This product meets the requirements of the following EMC standards for electrical equipment for measurement, control, and laboratory use:

- EN 61326-1 (IEC 61326-1): Class A emissions; Basic immunity
- EN 55011 (CISPR 11): Group 1, Class A emissions
- EN 55022 (CISPR 22): Class A emissions
- EN 55024 (CISPR 24): Immunity
- AS/NZS CISPR 11: Group 1, Class A emissions
- AS/NZS CISPR 22: Class A emissions
- FCC 47 CFR Part 15B: Class A emissions
- ICES-001: Class A emissions

**Note** In the United States (per FCC 47 CFR), Class A equipment is intended for use in commercial, light-industrial, and heavy-industrial locations. In Europe, Canada, Australia and New Zealand (per CISPR 11) Class A equipment is intended for use only in heavy-industrial locations.

**Note** Group 1 equipment (per CISPR 11) is any industrial, scientific, or medical equipment that does not intentionally generate radio frequency energy for the treatment of material or inspection/analysis purposes.

**Note** For EMC declarations and certifications, and additional information, refer to the *Online Product Certification* section.

# CE Compliance CE

This product meets the essential requirements of applicable European Directives as follows:

- 2014/35/EU; Low-Voltage Directive (safety)
- 2014/30/EU; Electromagnetic Compatibility Directive (EMC)

# Online Product Certification

Refer to the product Declaration of Conformity (DoC) for additional regulatory compliance information. To obtain product certifications and the DoC for this product, visit `ni.com/certification`, search by model number or product line, and click the appropriate link in the Certification column.



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

# Environmental Management

NI is committed to designing and manufacturing products in an environmentally responsible manner. NI recognizes that eliminating certain hazardous substances from our products is beneficial to the environment and to NI customers.

For additional environmental information, refer to the *Minimize Our Environmental Impact* web page at `ni.com/environment`. This page contains the environmental regulations and directives with which NI complies, as well as other environmental information not included in this document.

## Waste Electrical and Electronic Equipment (WEEE)



**EU Customers** At the end of the product life cycle, all products *must* be sent to a WEEE recycling center. For more information about WEEE recycling centers, National Instruments WEEE initiatives, and compliance with WEEE Directive 2002/96/EC on Waste and Electronic Equipment, visit `ni.com/environment/weee`.

## 电子信息产品污染控制管理办法 （中国 RoHS）



**中国客户** National Instruments 符合中国电子信息产品中限制使用某些有害物质指令 (RoHS)。关于 National Instruments 中国 RoHS 合规性信息，请登录 `ni.com/environment/rohs_china`。 (For information about China RoHS compliance, go to `ni.com/environment/rohs_china`.)

# World Wide Support and Services

The National Instruments website is your complete resource for technical support. At `ni.com/support` you have access to everything from troubleshooting and application development self-help resources to email and phone assistance from NI Application Engineers.

Visit `ni.com/services` for NI Factory Installation Services, repairs, extended warranty, and other services.

Visit `ni.com/register` to register your National Instruments product. Product registration facilitates technical support and ensures that you receive important information updates from NI.

National Instruments corporate headquarters is located at 11500 North Mopac Expressway, Austin, Texas, 78759-3504. National Instruments also has offices located around the world. For telephone support in the United States, create your service request at `ni.com/support` or dial 1 866 ASK MYNI (275 6964). For telephone support outside the United States, visit the Worldwide Offices section of `ni.com/niglobal` to access the branch office websites, which provide up-to-date contact information, support phone numbers, email addresses, and current events.



Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

Refer to the *NI Trademarks and Logo Guidelines* at `ni.com/trademarks` for more information on NI trademarks. Other product and company names mentioned herein are trademarks or trade names of their respective companies. For patents covering NI products/technology, refer to the appropriate location: **Help»Patents** in your software, the `patents.txt` file on your media, or the *National Instruments Patents Notice* at `ni.com/patents`. You can find information about end-user license agreements (EULAs) and third-party legal notices in the readme file for your NI product. Refer to the *Export Compliance Information* at `ni.com/legal/export-compliance` for the NI global trade compliance policy and how to obtain relevant HTS codes, ECCNs, and other import/export data. NI MAKES NO EXPRESS OR IMPLIED WARRANTIES AS TO THE ACCURACY OF THE INFORMATION CONTAINED HEREIN AND SHALL NOT BE LIABLE FOR ANY ERRORS. U.S. Government Customers: The data contained in this manual was developed at private expense and is subject to the applicable limited rights and restricted data rights as set forth in FAR 52.227-14, DFAR 252.227-7014, and DFAR 252.227-7015.

© 2015–2016 National Instruments. All rights reserved.

37007B-01 May16

Artisan Technology Group - Quality Instrumentation ... Guaranteed | (888) 88-SOURCE | www.artisantg.com

**Artisan Technology Group** is an independent supplier of quality pre-owned equipment

## Gold-standard solutions

Extend the life of your critical industrial, commercial, and military systems with our superior service and support.

## We buy equipment

Planning to upgrade your current equipment? Have surplus equipment taking up shelf space? We'll give it a new home.

## Learn more!

Visit us at **artisantg.com** for more info on price quotes, drivers, technical specifications, manuals, and documentation.

Artisan Scientific Corporation dba Artisan Technology Group is not an affiliate, representative, or authorized distributor for any manufacturer listed herein.

We're here to make your life easier. How can we help you today?

(217) 352-9330 | sales@artisantg.com | artisantg.com

ARTISAN® TECHNOLOGY GROUP